




Pile Dynamics, Inc.

Transducer B981

Strain ($\mu\epsilon$)

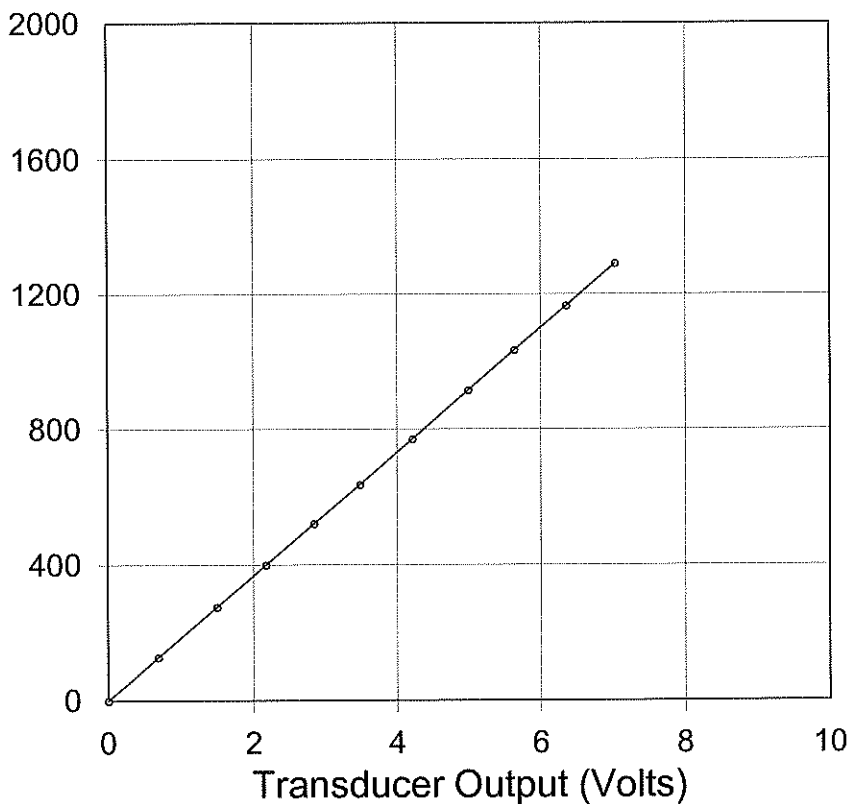

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

PDA Cal Factor (5.0 V)

91.5 $\mu\epsilon$ /V

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
128	0.68
277	1.49
398	2.17
520	2.84
634	3.48
769	4.21
914	4.99
1033	5.63
1165	6.35
1291	7.03

Shunt (60.4 K Ω)

2.5 V

General Factor

317.8 $\mu\epsilon$ /mV/V

Calibrated by:

Calibrated on:

04-Dec-2007