




Pile Dynamics, Inc.

Transducer B982

Strain ($\mu\epsilon$)

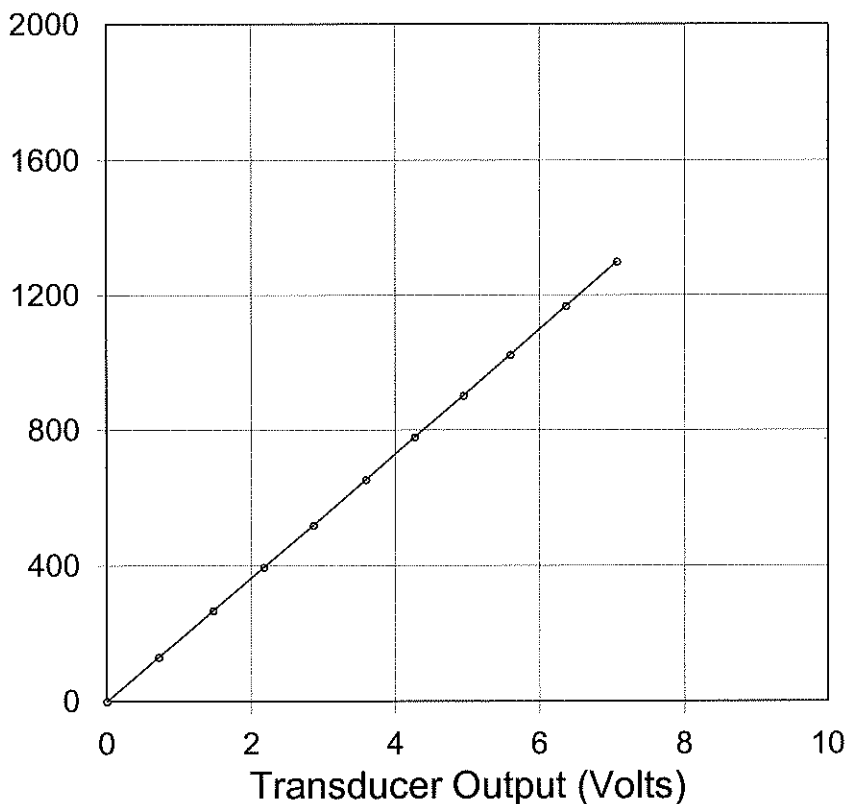

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

PDA Cal Factor (5.0 V)

91.8 $\mu\epsilon$ /V

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
131	0.71
268	1.46
396	2.17
517	2.86
653	3.59
778	4.27
902	4.94
1023	5.59
1168	6.36
1300	7.07

Shunt (60.4 K Ω)

2.5 V

General Factor

318.9 $\mu\epsilon$ /mV/V

Calibrated by:

Calibrated on:

04-Dec-2007