




Pile Dynamics, Inc.

Transducer B988

Strain ($\mu\epsilon$)

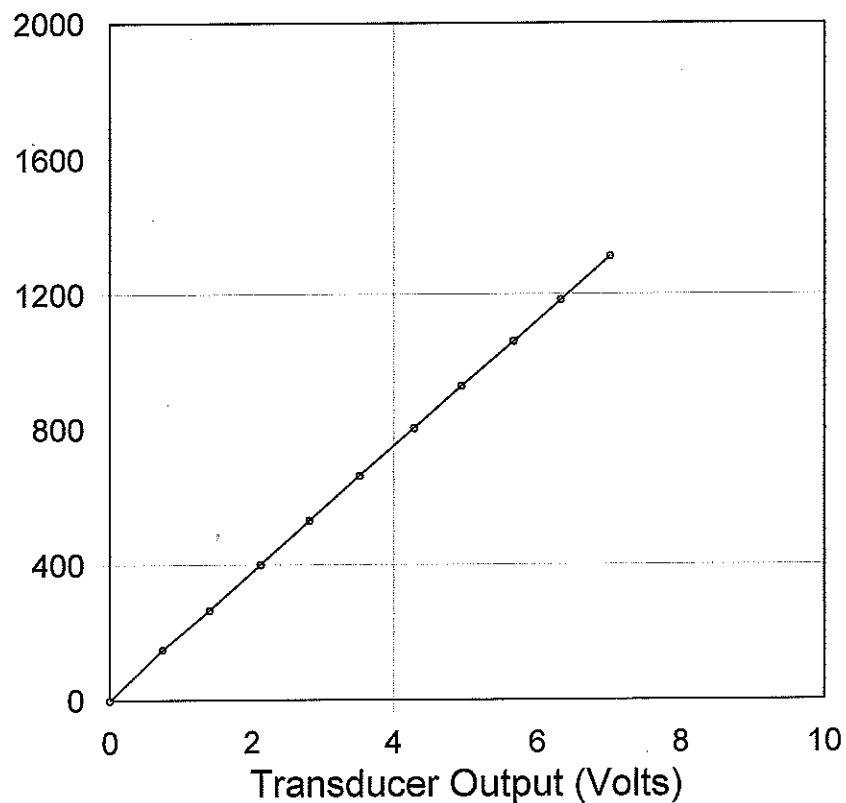

PDA Cal Factor (5.0 V)

93.2 $\mu\epsilon$ /V

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
151	0.74
264	1.40
398	2.11
529	2.81
660	3.52
802	4.28
929	4.94
1060	5.66
1183	6.32
1312	7.01

Shunt (60.4 K Ω)

2.5 V

General Factor

323.6 $\mu\epsilon$ /mV/V

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

Calibrated by:

Calibrated on:

Ej. Singh
19-Feb-2013