




Pile Dynamics, Inc.

Transducer

B989

Strain ($\mu\epsilon$)

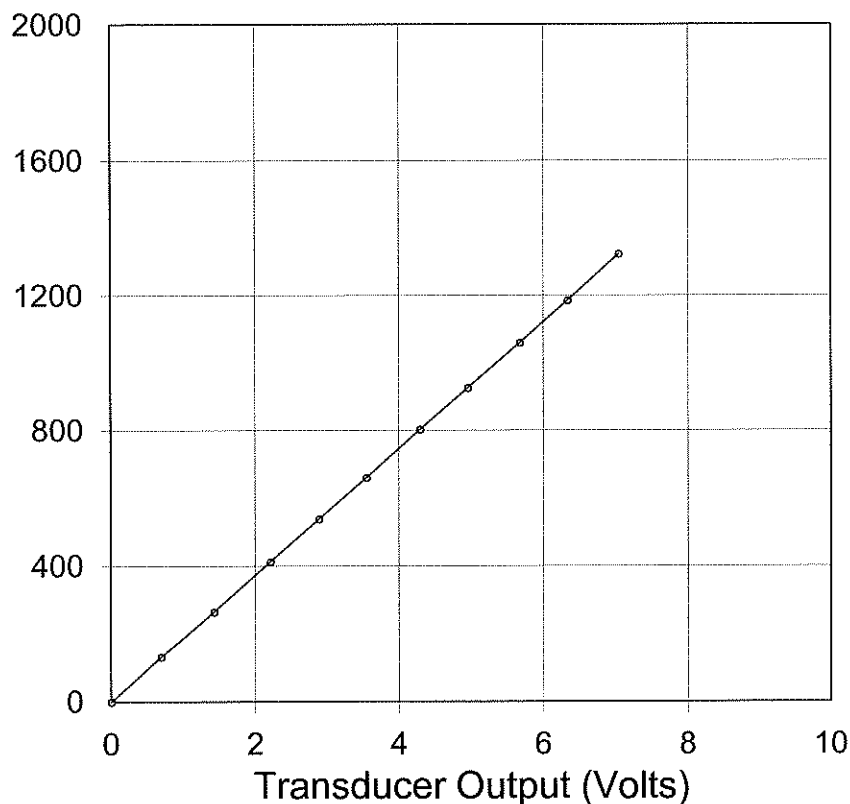

PDA Cal Factor (5.0 V)

93.7 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
133	0.69
266	1.42
412	2.21
538	2.89
659	3.55
801	4.29
925	4.95
1060	5.67
1186	6.33
1323	7.04

Shunt (60.4 K Ω)

2.5 V

General Factor

325.4 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

Calibrated by:

Calibrated on:

S. Hall
04-Dec-2007