




Pile Dynamics, Inc.

Transducer B990

Strain ($\mu\epsilon$)

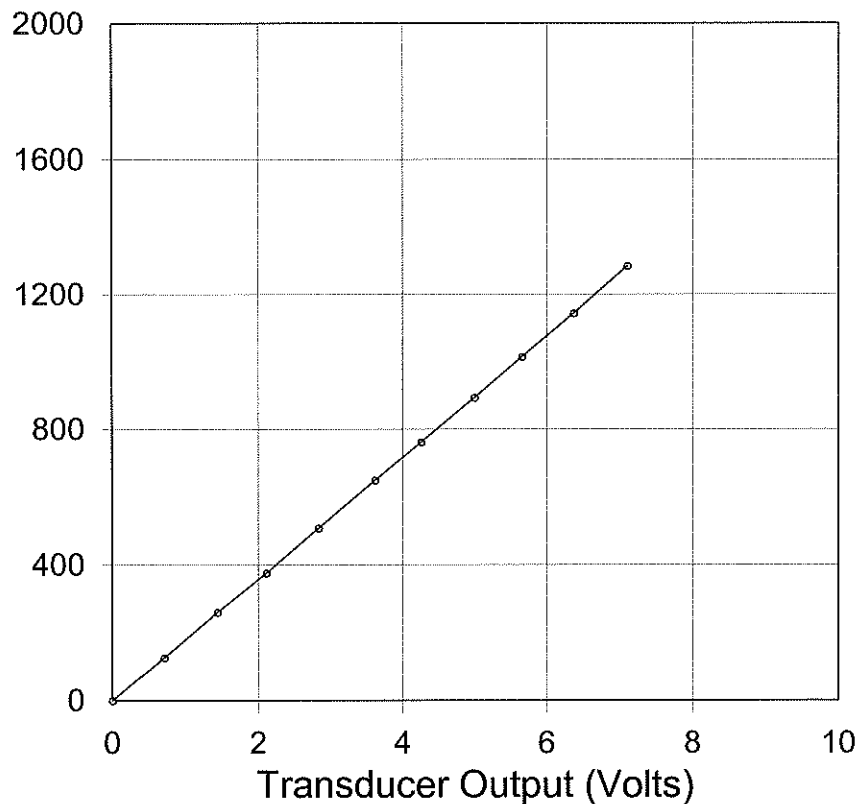

PDA Cal Factor (5.0 V)

90.0 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
126	0.70
261	1.43
375	2.11
508	2.83
648	3.61
760	4.25
893	4.99
1014	5.65
1145	6.36
1284	7.10

Shunt (60.4 K Ω)

2.5 V

General Factor

312.6 $\mu\epsilon/mV/V$

Calibrated by:

Calibrated on:

[Signature]

18-Dec-2007

Traceable to N.I.S.T.