




Pile Dynamics, Inc.

Transducer B996

Strain ($\mu\epsilon$)

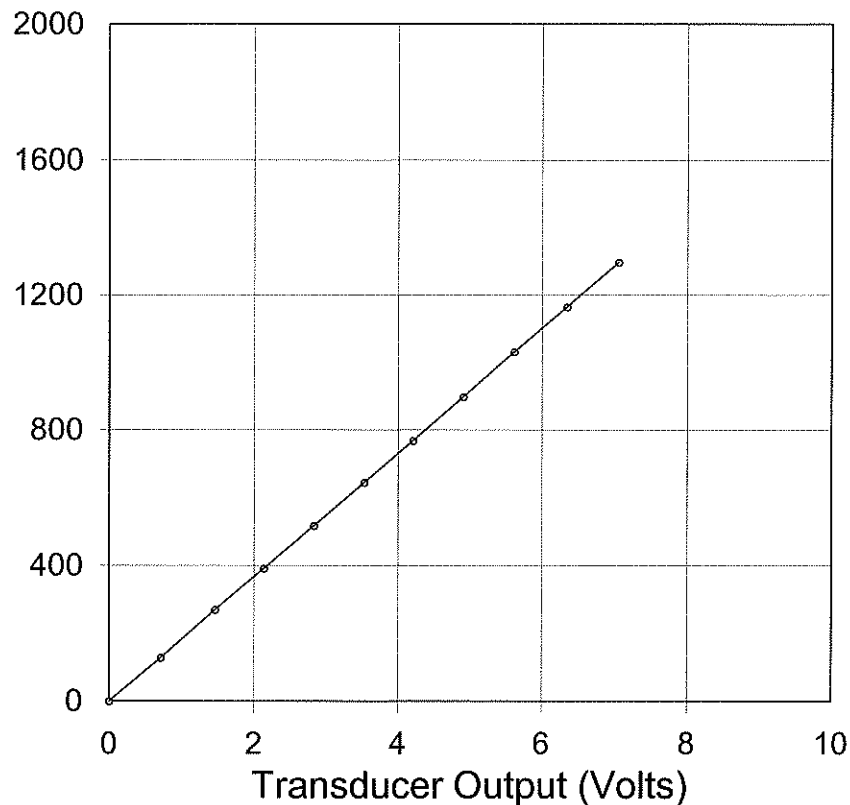

PDA Cal Factor (5.0 V)

91.9 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
129	0.70
270	1.45
390	2.13
516	2.82
643	3.52
768	4.20
897	4.90
1031	5.61
1167	6.34
1298	7.05

Shunt (60.4 K Ω)

2.5 V

General Factor

319.1 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

Calibrated by:

Calibrated on:

03-Jan-2008