




Pile Dynamics, Inc.

Transducer B997

Strain ($\mu\epsilon$)

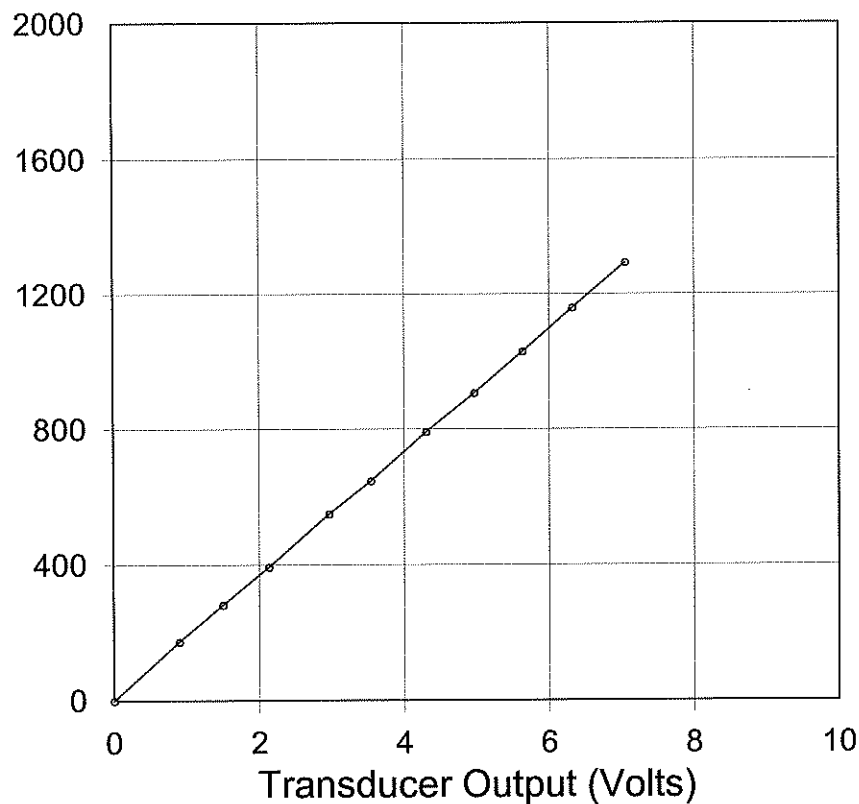

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

PDA Cal Factor (5.0 V)

91.1 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
174	0.89
282	1.49
392	2.13
548	2.96
647	3.54
791	4.31
906	4.96
1029	5.63
1160	6.32
1293	7.05

Shunt (60.4 K Ω)

2.5 V

General Factor

316.5 $\mu\epsilon/mV/V$

Calibrated by:

Calibrated on:

18-Feb-2008