


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

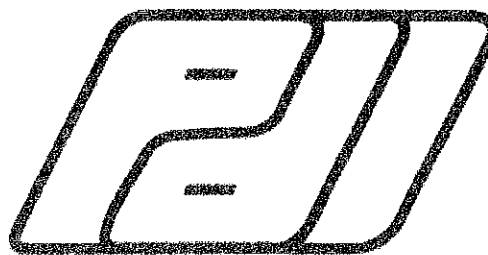

Serial No: 22331 Temperature: 22.3 °C

Model: PE Humidity: 28%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR


1040.4 g's/volt

R²: 0.999966 [No chip]

Ref Acc 1: 78268! Cal on: 11Jan2024
986 g's/volt

Ref Acc 2: 78270! Cal on: 11Jan2024
971 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 14Nov2025

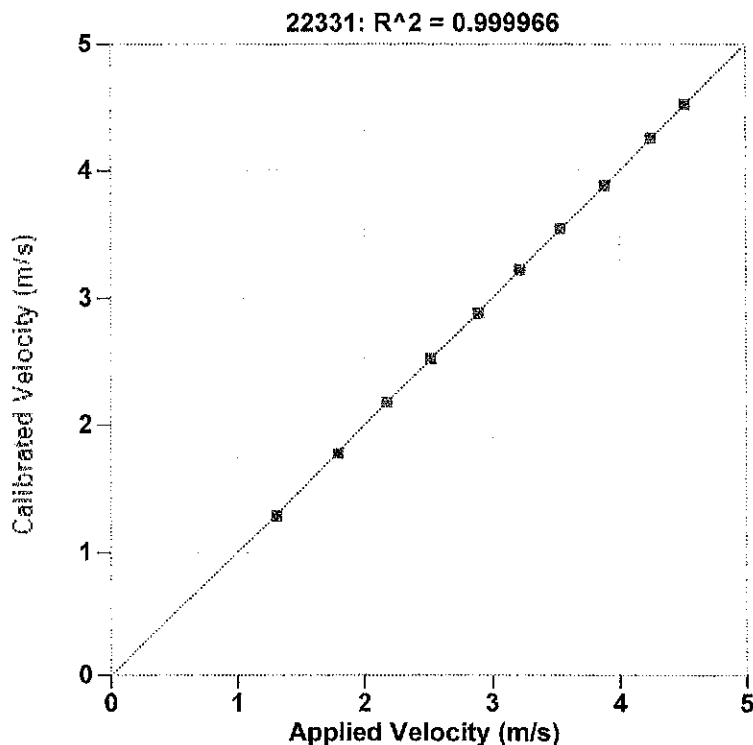

Reference Velocity	S/N 22331 Velocity
m/s	m/s
1.306	1.298
1.794	1.783
2.184	2.184
2.523	2.528
2.894	2.888
3.225	3.225
3.541	3.549
3.890	3.888
4.253	4.257
4.523	4.523
Maximum Acceleration: 979 g's	