


Cycle 1
Sample

	Force (kips)	Bridge (mV/V)
1	0	0
2	1.08832466	0.064097909
3	2.00284872	0.117329596
4	2.97849051	0.174082265
5	3.99380525	0.232104958
6	5.07657382	0.292625049
7	6.14881513	0.353292066
8	6.91907446	0.394368608
9	8.05418867	0.457168168
10	8.8256182	0.499429469
11	10.0252628	0.564451633

Serial Number 30042DC
Force Calibration (lb/V) 17.8741774
Offset -0.11718838
Correlation 0.99992121

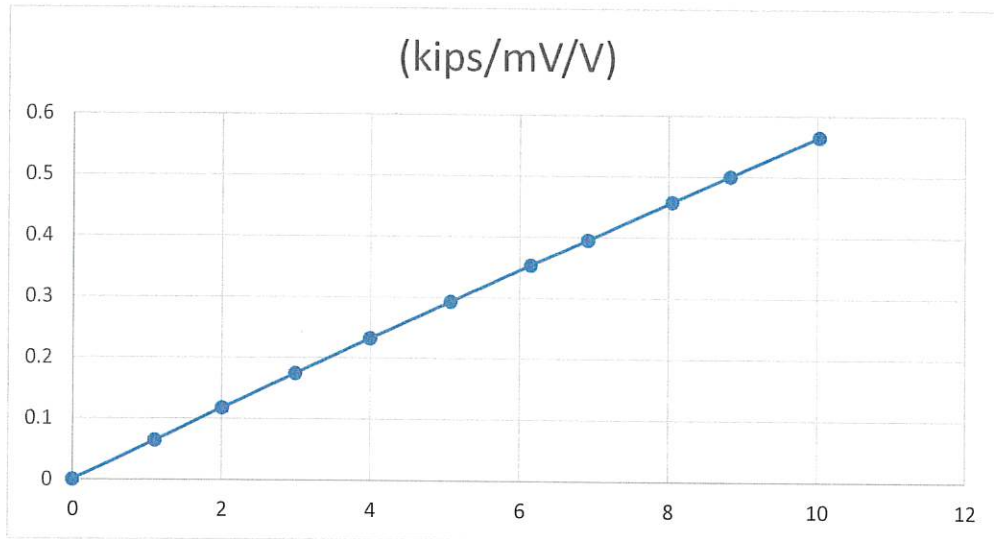


Cycle 2
Sample

	Force (kips)	Bridge (mV/V)
1	0	0
2	1.05605996	0.04988131
3	1.95752218	0.096767655
4	2.92682799	0.149482806
5	3.96202793	0.20610279


6	5.02120718	0.265239124
7	6.14569587	0.32859307
8	6.91381072	0.36989707
9	8.08294422	0.434805414
10	8.87718327	0.478450457
11	10.0779976	0.544865835

Serial Number	30042DC
Force Calibration (kips/mV/V)	18.1568867
Offset	0.1928987
Correlation	0.9999793

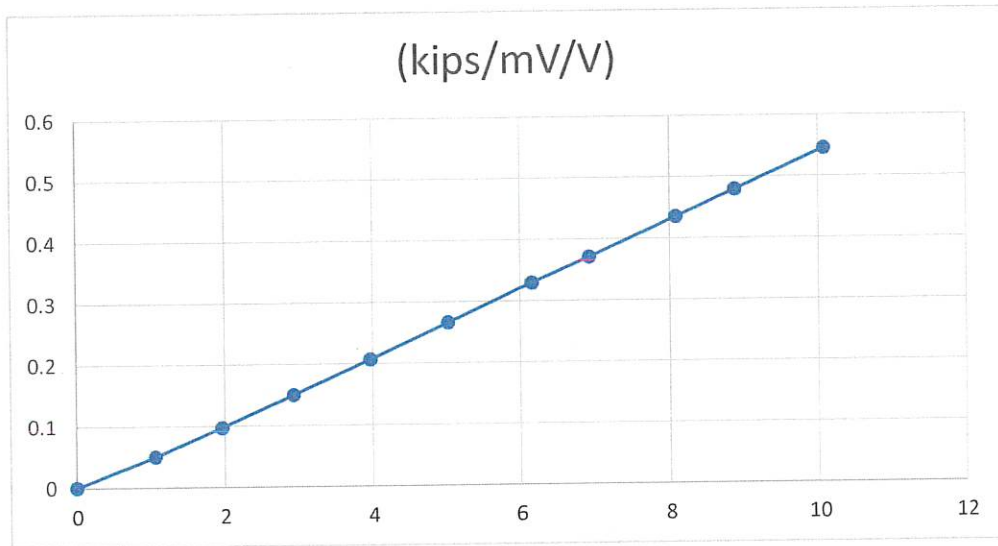

Sample	Cycle 3	
	Force (kips)	Bridge (mV/V)
1	0	0
2	1.16611088	0.060548497
3	2.10071509	0.110311334
4	3.0547171	0.16139158
5	4.10668299	0.218584974
6	5.19549511	0.277944045
7	5.91204472	0.318087014
8	7.06207248	0.380346313
9	8.21229559	0.444074698
10	9.01988896	0.486757763
11	9.99962631	0.542131573

Serial Number 30042DC
Force Calibration (kips/mV/V) 18.3314446
Offset 0.08320564
Correlation 0.99998564

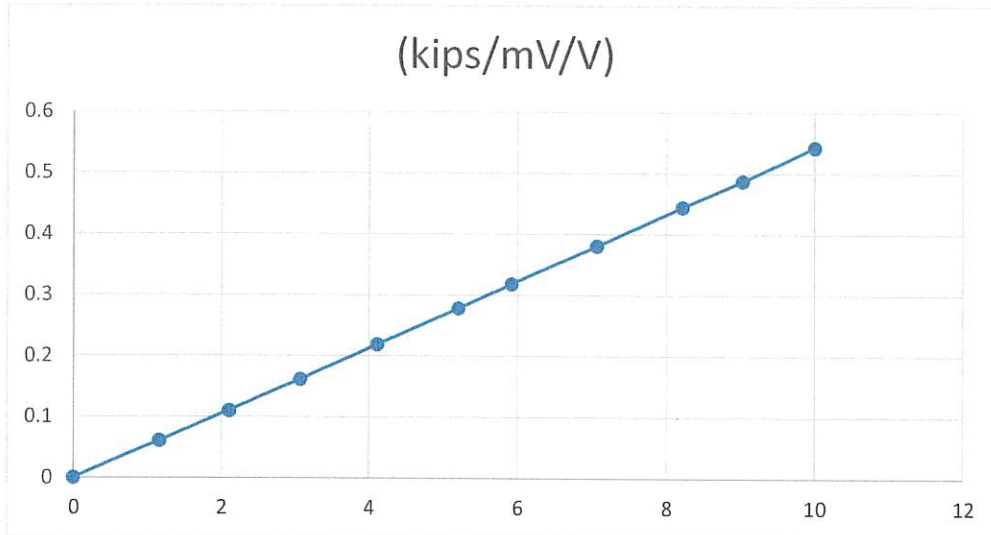

Serial Number 30042DC
Force Calibration (kips/mV/V) 18.1208362

Squid Gain 50
Squid Excitation 5
Force Calibration (kips/V) 3624.16725

Calibrated by: Sean Bonney
Calibrated Date: 1/13/2025

Pile Dynamics Inc
30725 Aurora Rd
Solon, OH 44139

Traceable to N.I.S.T.

