


Cycle 1  
Sample

| Force (kips)  | Bridge (mV/V) |
|---------------|---------------|
| 1 0           | 0             |
| 2 0.88781559  | 0.054354799   |
| 3 1.98920201  | 0.121485582   |
| 4 2.93940244  | 0.177276263   |
| 5 3.93502694  | 0.236872264   |
| 6 4.95199889  | 0.297453967   |
| 7 5.96331738  | 0.357594978   |
| 8 7.11480735  | 0.424768507   |
| 9 7.88263     | 0.468925351   |
| 10 9.00984902 | 0.535009014   |
| 11 9.79560794 | 0.581416884   |

Serial Number 30043DC  
 Force Calibration (lb/V) 16.9297808  
 Offset -0.06394472  
 Correlation 0.99998178

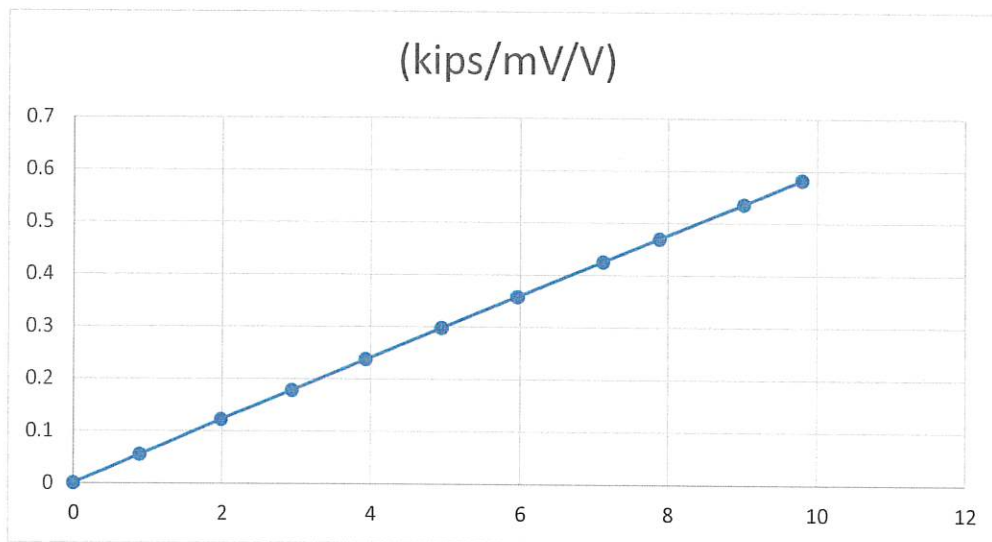


Cycle 2  
Sample

| Force (kips) | Bridge (mV/V) |
|--------------|---------------|
| 1 0          | 0             |
| 2 1.13579571 | 0.061008168   |
| 3 2.00080174 | 0.108870725   |
| 4 3.16749736 | 0.17406333    |
| 5 4.10083441 | 0.226802205   |


|    |            |             |
|----|------------|-------------|
| 6  | 5.07832839 | 0.280005507 |
| 7  | 6.15807537 | 0.339331455 |
| 8  | 7.2686252  | 0.401007919 |
| 9  | 8.00311087 | 0.440994571 |
| 10 | 9.16006022 | 0.504623525 |
| 11 | 9.917161   | 0.546505784 |

Serial Number 30043DC  
 Force Calibration (kips/mV/V) 18.0977625  
 Offset 0.01910301  
 Correlation 0.99999335

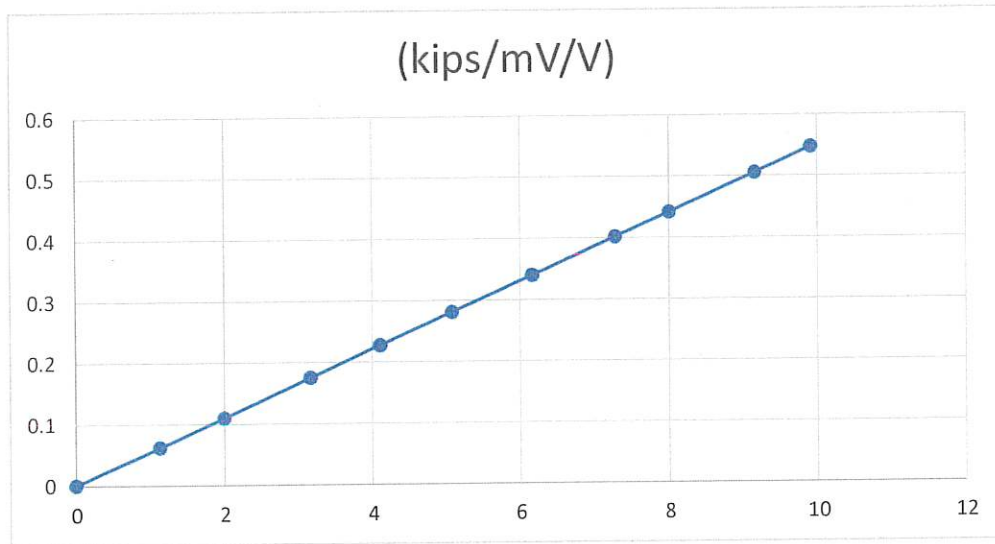

| Sample | Cycle 3      |               |
|--------|--------------|---------------|
|        | Force (kips) | Bridge (mV/V) |
| 1      | 0            | 0             |
| 2      | 0.95215006   | 0.057003832   |
| 3      | 2.15393722   | 0.127750394   |
| 4      | 2.87146137   | 0.170722462   |
| 5      | 3.88092751   | 0.229470245   |
| 6      | 5.01223935   | 0.296373659   |
| 7      | 6.07824214   | 0.358301295   |
| 8      | 7.04940055   | 0.412945313   |
| 9      | 7.91547952   | 0.462111218   |
| 10     | 8.99054855   | 0.522370894   |
| 11     | 10.1308299   | 0.585672996   |

Serial Number 30043DC  
Force Calibration (kips/mV/V) 17.3358469  
Offset -0.08334045  
Correlation 0.99992772

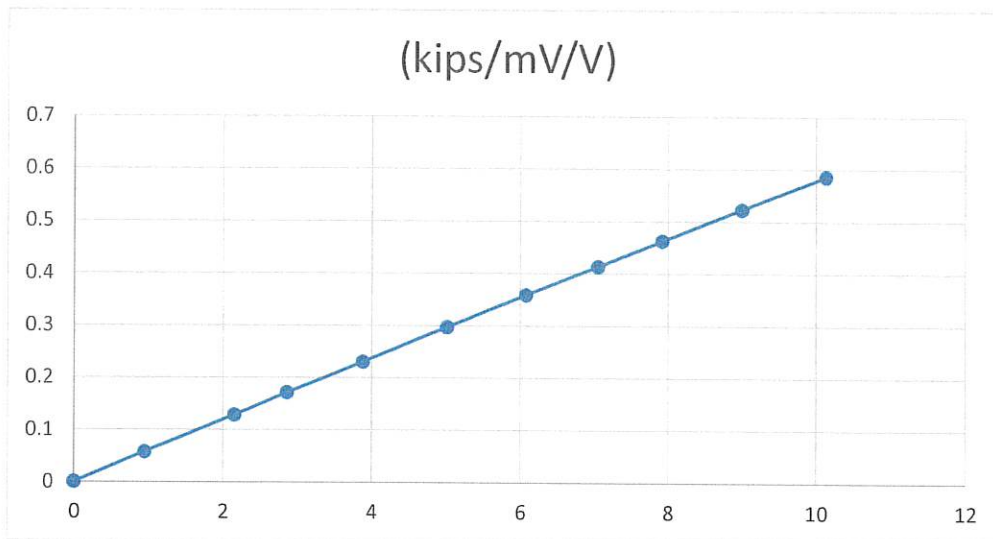

Serial Number 30043DC  
Force Calibration (kips/mV/V) 17.4544634

Squid Gain 50  
Squid Excitation 5  
Force Calibration (kips/V) 3490.89268

Calibrated by: Sean Bonner  
Calibrated Date: 1/13/2025

Pile Dynamics Inc  
30725 Aurora Rd  
Solon, OH 44139

Traceable to N.I.S.T.

