


6	4.87178464	-0.275841949
7	5.91546634	-0.335642288
8	6.99648145	-0.398148609
9	8.12087354	-0.462351535
10	8.86978591	-0.506788459
11	9.84172462	-0.565655476

Serial Number	30382
Force Calibration (kips/mV/V)	-17.423928
Offset	0.04093686
Correlation	-0.99996014

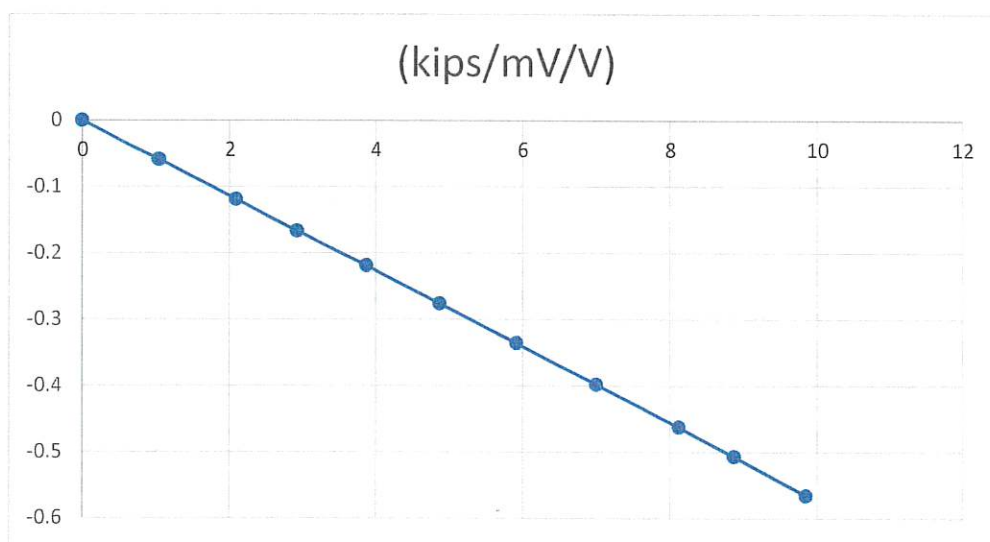


Sample	Cycle 3	
	Force (kips)	Bridge (mV/V)
1	0	0
2	1.08345333	-0.060634165
3	2.14624128	-0.121704356
4	3.02401832	-0.171287494
5	4.26148384	-0.2424327
6	5.31598556	-0.30142267
7	6.01294306	-0.342584889
8	7.10097649	-0.403712212
9	8.19914738	-0.468469621
10	8.95537049	-0.511589143
11	10.0200094	-0.571195461

Cycle 1
Sample

	Force (kips)	Bridge (mV/V)
1	0	0
2	1.03130331	-0.058923409
3	2.19000828	-0.124405497
4	3.10073241	-0.176258557
5	4.12647874	-0.233864688
6	5.18409973	-0.293347478
7	6.24503476	-0.353470078
8	6.99755384	-0.396707966
9	8.09864903	-0.459773546
10	9.11581688	-0.524393568
11	10.0686502	-0.569830459


Serial Number 30382
 Force Calibration (lb/V) -17.5615064
 Offset 0.01199949
 Correlation -0.99990545

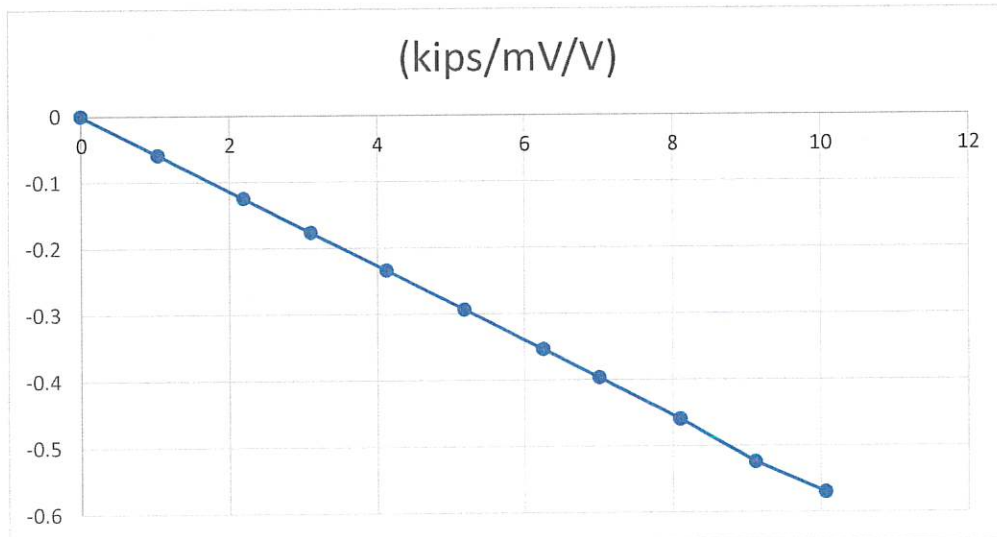

Cycle 2
Sample

	Force (kips)	Bridge (mV/V)
1	0	0
2	1.03841907	-0.058454259
3	2.08824261	-0.118690388
4	2.93112301	-0.166425338
5	3.86660603	-0.218714409

Serial Number 30382
Force Calibration (kips/mV/V) -17.4809942
Offset 0.02672807
Correlation -0.99999163

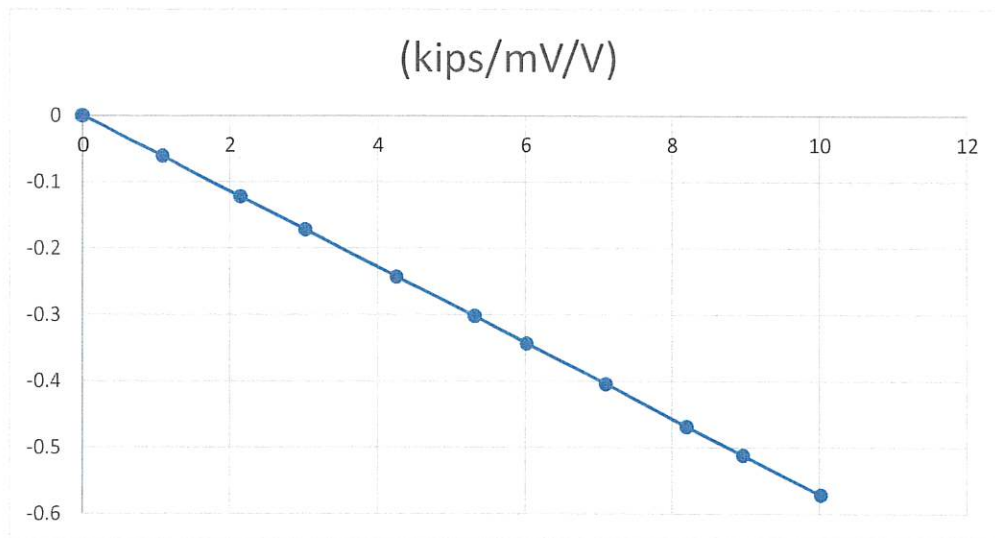

Serial Number 30382
Force Calibration (kips/mV/V) -17.4888096
Squid Gain 50
Squid Excitation 5
Force Calibration (kips/V) -3497.76191

Calibrated by: Sean Benner
Calibrated Date: 7/11/2024

Pile Dynamics Inc
30725 Aurora Rd
Solon, OH 44139

Traceable to N.I.S.T.

