


Cycle 1
Sample

Force (kips)	Bridge (mV/V)
1 0	0
2 1.11123418	-0.062093628
3 2.24254819	-0.124917084
4 3.18300268	-0.177736779
5 4.175412	-0.235181671
6 5.24053868	-0.295398862
7 5.95289749	-0.334854963
8 7.12680777	-0.401123824
9 8.28648637	-0.467800299
10 9.04621863	-0.511189805
11 10.0237135	-0.566834192

Serial Number 30384
Force Calibration (lb/V) -17.6431791
Offset 0.03341663
Correlation -0.99999284

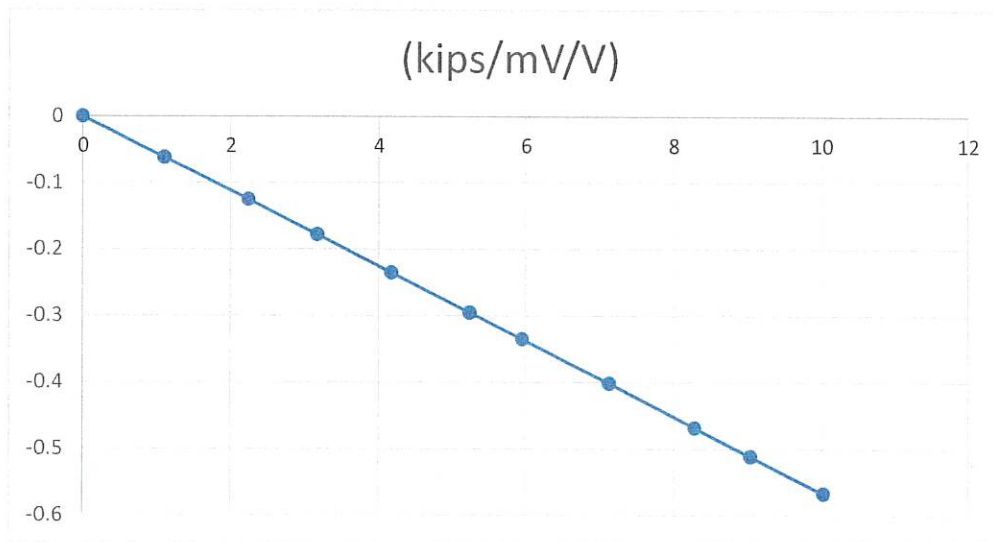


Cycle 2
Sample

Force (kips)	Bridge (mV/V)
1 0	0
2 1.12117677	-0.063714394
3 1.95986588	-0.111880517
4 2.87380677	-0.163463415
5 3.88444425	-0.220060107


6	4.93017312	-0.27914951
7	6.04501272	-0.34186897
8	7.1685276	-0.406683095
9	7.92328858	-0.450546521
10	9.11991076	-0.518914962
11	9.89894338	-0.565607619

Serial Number 30384
 Force Calibration (kips/mV/V) -17.5440608
 Offset 0.01545375
 Correlation -0.99997672

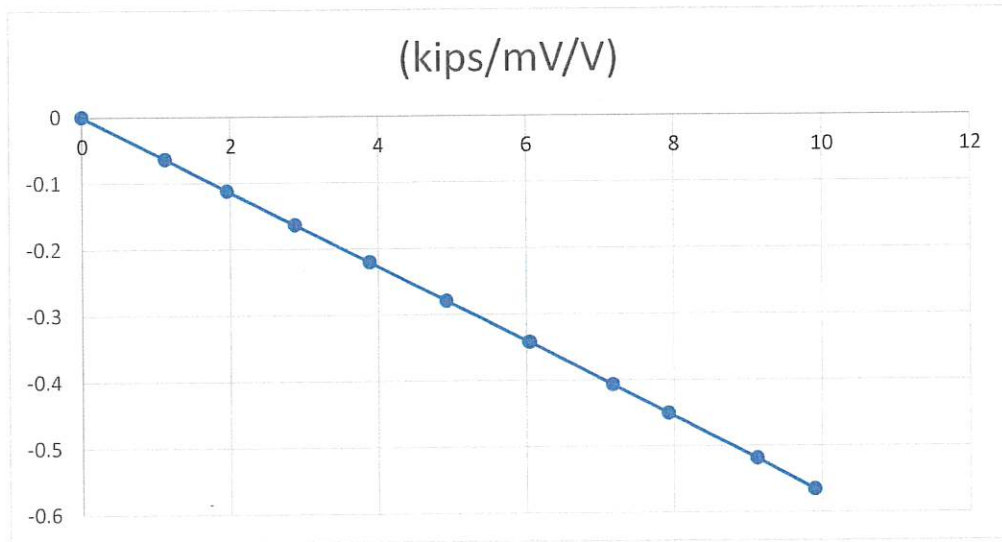

Sample	Cycle 3	
	Force (kips)	Bridge (mV/V)
1	0	0
2	1.11484079	-0.062918308
3	2.00499758	-0.11259144
4	2.96143827	-0.167567438
5	4.00190358	-0.225590597
6	5.05338356	-0.286367115
7	6.16666351	-0.349129299
8	6.92347156	-0.392386149
9	8.07047822	-0.456802333
10	8.87037082	-0.502480861
11	10.0278074	-0.570494033

Serial Number 30384
Force Calibration (kips/mV/V) -17.5884343
Offset 0.02081482
Correlation -0.9999905

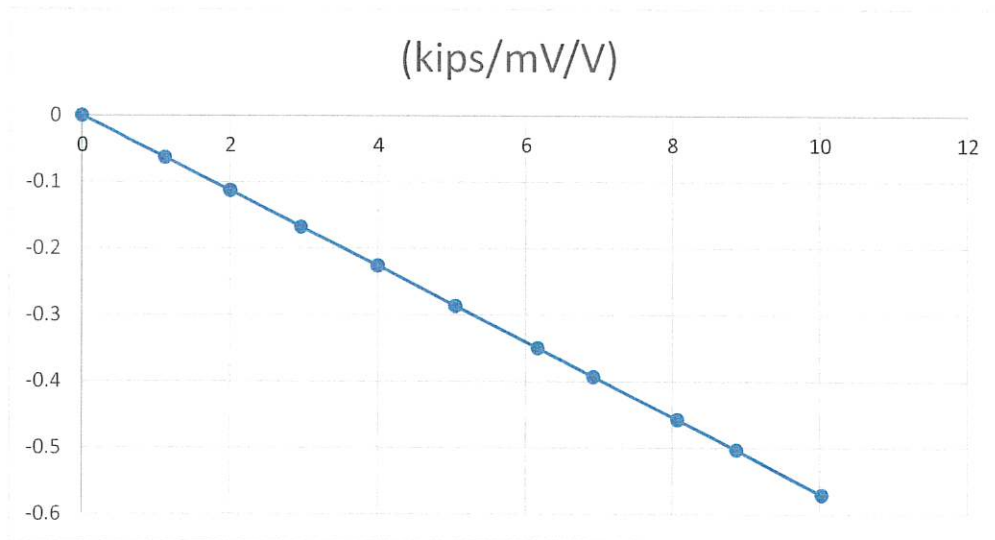

Serial Number 30384
Force Calibration (kips/mV/V) -17.5918914

Squid Gain 50
Squid Excitation 5
Force Calibration (kips/V) -3518.37828

Calibrated by: Sean Bone
Calibrated Date: 7/11/2024

Pile Dynamics Inc
30725 Aurora Rd
Solon, OH 44139

Traceable to N.I.S.T.

