


Cycle 1
Sample

Force (kips)	Bridge (mV/V)
1 0	0
2 1.10207135	-0.061890179
3 1.98647701	-0.11231224
4 2.9529578	-0.16653496
5 3.95979369	-0.223487354
6 5.04334346	-0.284984446
7 6.14414642	-0.346912856
8 6.90329391	-0.390046694
9 8.08207792	-0.457178607
10 8.85253261	-0.501317208
11 10.0446709	-0.570126883

Serial Number 30385
Force Calibration (lb/V) -17.6246513
Offset 0.01742523
Correlation -0.9999942

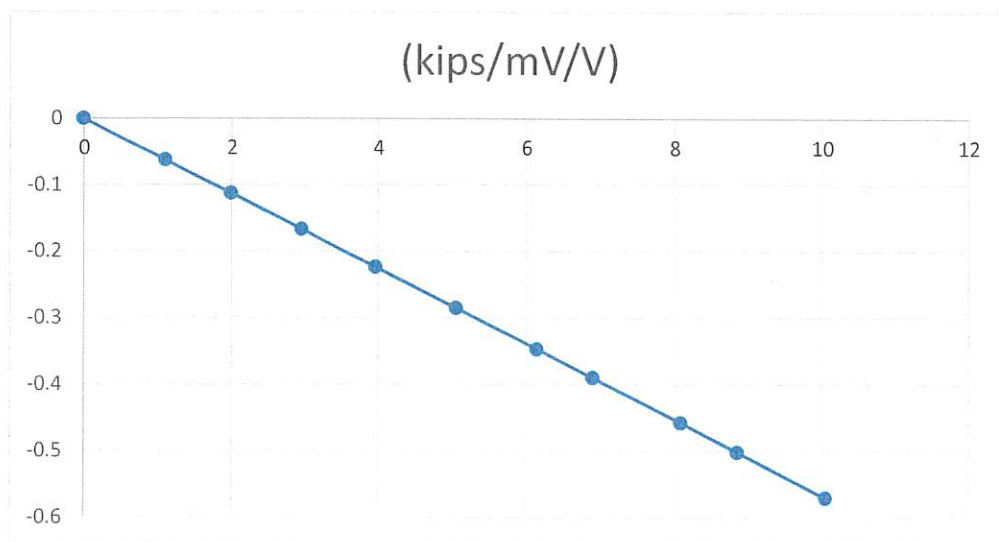


Cycle 2
Sample

Force (kips)	Bridge (mV/V)
1 0	0
2 1.07224351	-0.060293419
3 2.24137847	-0.126681187
4 3.21994632	-0.18252963
5 4.27347346	-0.241581673


6	4.96984621	-0.281327282
7	6.09297132	-0.344985732
8	7.22652629	-0.408762754
9	8.00136745	-0.453451277
10	9.19906187	-0.522024329
11	9.98004402	-0.5673954

Serial Number 30385
 Force Calibration (kips/mV/V) -17.5943105
 Offset 0.01680278
 Correlation -0.99999403

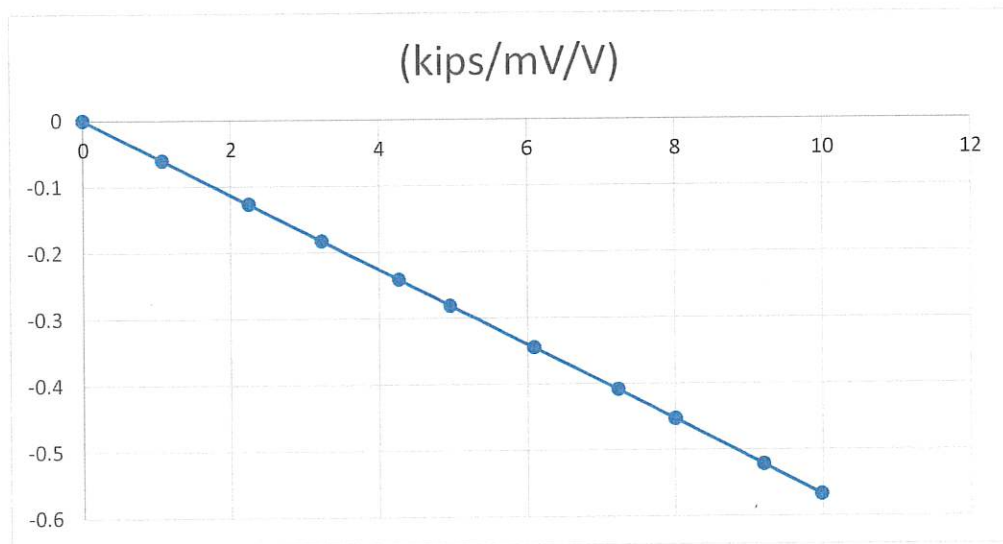

Sample	Cycle 3	
	Force (kips)	Bridge (mV/V)
1	0	0
2	0.83712974	-0.048048125
3	2.00197576	-0.113497722
4	2.98181081	-0.16856436
5	4.00326817	-0.226720873
6	5.07999457	-0.287938843
7	5.8230585	-0.33034317
8	6.94706078	-0.393916575
9	8.1282817	-0.461451885
10	8.90458497	-0.505770964
11	10.1082255	-0.574102639

Serial Number 30385
Force Calibration (kips/mV/V) -17.6067494
Offset 0.00521466
Correlation -0.99999739

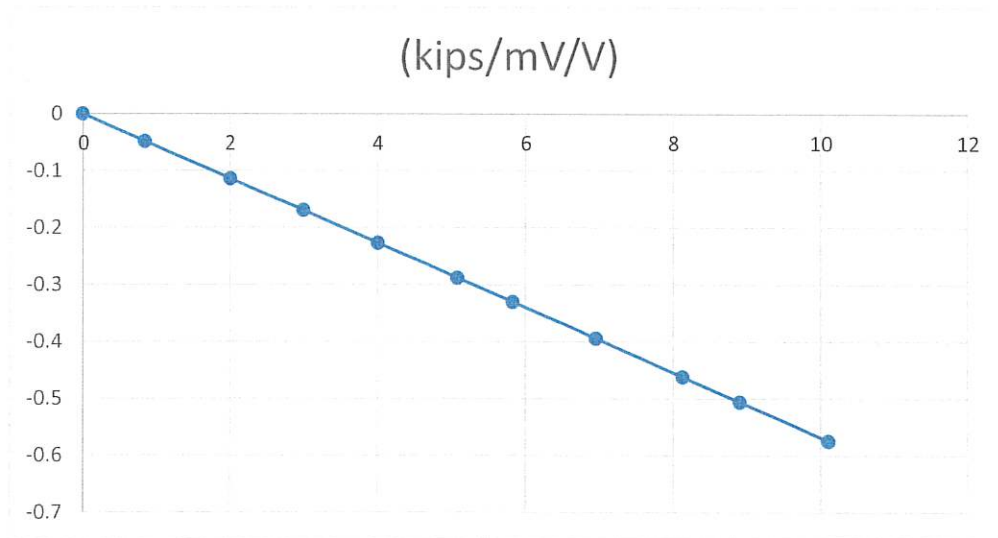

Serial Number 30385
Force Calibration (kips/mV/V) -17.6085704

Squid Gain 50
Squid Excitation 5
Force Calibration (kips/V) -3521.71408

Calibrated by: Sean Bonner
Calibrated Date: 7/11/2024

Pile Dynamics Inc
30725 Aurora Rd
Solon, OH 44139

Traceable to N.I.S.T.

