


Cycle 1
Sample

	Force (kips)	Bridge (mV/V)
1	0	0
2	0.999136	-0.057724725
3	2.06348359	-0.118103304
4	3.06086445	-0.174363821
5	4.10396162	-0.233790004
6	5.22299286	-0.297012148
7	5.95845362	-0.338729045
8	7.13041436	-0.404590923
9	8.1373472	-0.462804223
10	9.15821914	-0.523510295
11	9.99378816	-0.564327005

Serial Number 30388
Force Calibration (lb/V) -17.6481399
Offset -0.02033976
Correlation -0.9999587

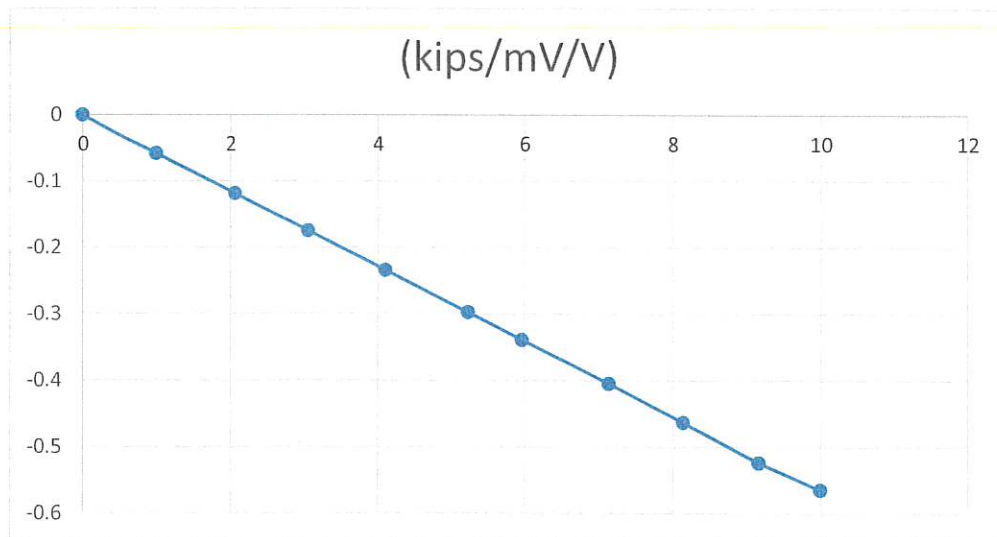


Cycle 2
Sample

	Force (kips)	Bridge (mV/V)
1	0	0
2	0.98812114	-0.054701301
3	2.22149322	-0.125913062
4	2.97742447	-0.169857119
5	3.93678926	-0.223407027


6	5.02959932	-0.285411258
7	6.17163488	-0.349856124
8	6.9655815	-0.394658131
9	7.92874737	-0.448350461
10	9.36525935	-0.535499939
11	10.2188615	-0.586036294

Serial Number 30388
 Force Calibration (kips/mV/V) -17.4639059
 Offset 0.03784761
 Correlation -0.99994146

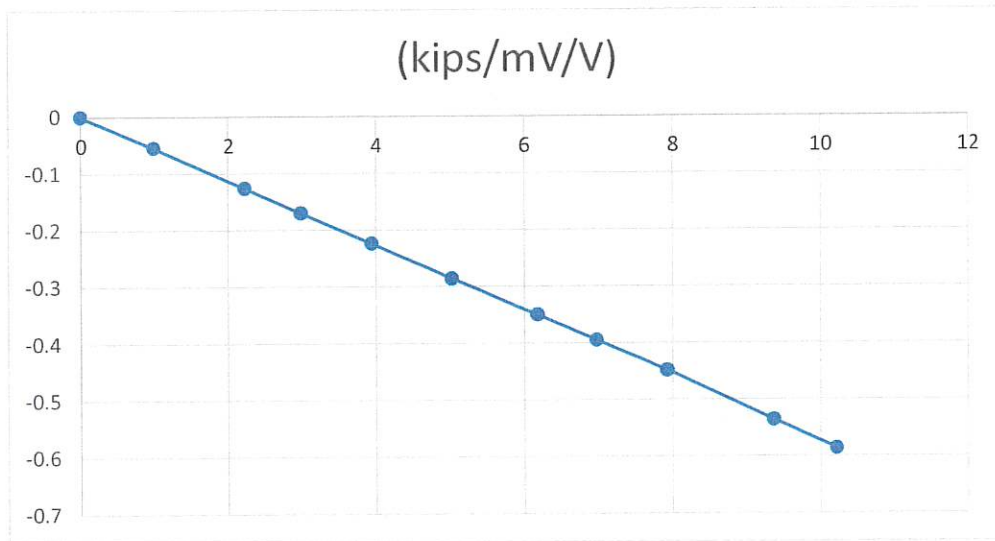

Sample	Cycle 3	
	Force (kips)	Bridge (mV/V)
1	0	0
2	1.09710007	-0.061724383
3	1.98686697	-0.113051634
4	2.973233	-0.167065905
5	4.03475328	-0.227359317
6	5.12112987	-0.289861147
7	6.24854393	-0.354050123
8	7.04551233	-0.398880573
9	8.19193412	-0.465012676
10	8.99348382	-0.510283963
11	10.0589026	-0.578771511

Serial Number 30388
Force Calibration (kips/mV/V) -17.462337
Offset 0.04646319
Correlation -0.9999113

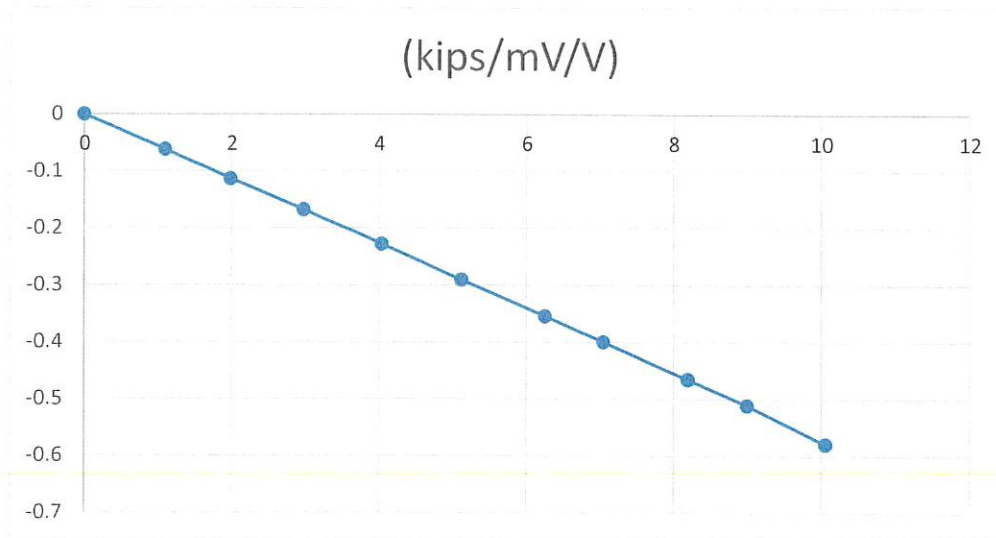

Serial Number 30388
Force Calibration (kips/mV/V) -17.5247942
Squid Gain 50
Squid Excitation 5
Force Calibration (kips/V) -3504.95885

Calibrated by: Jason Banner
Calibrated Date: 7/30/2024

Pile Dynamics Inc
30725 Aurora Rd
Solon, OH 44139

Traceable to N.I.S.T.

