


Serial Number 30399
Force Calibration (kips/mV/V) -17.349205
Offset 0.01030503
Correlation -0.9999871

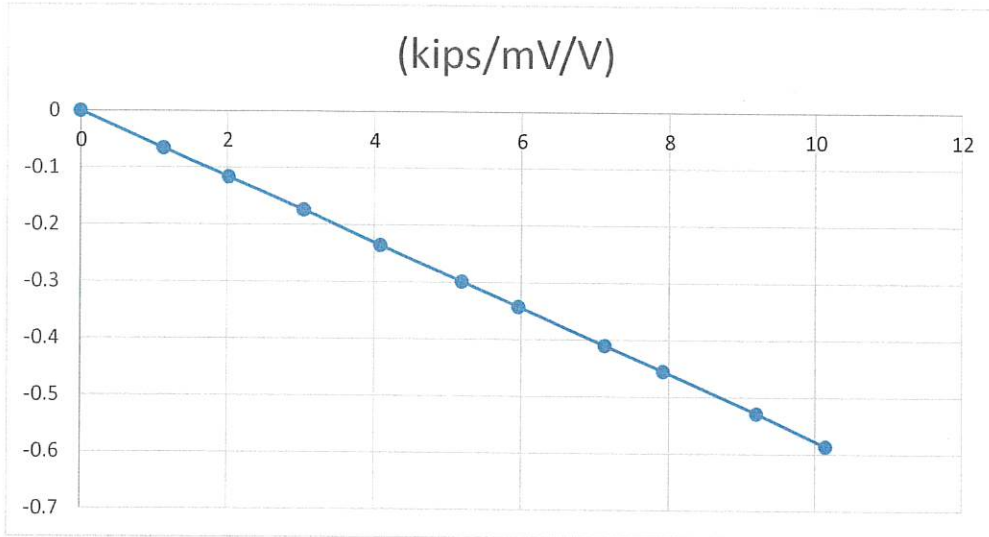

Serial Number 30399
Force Calibration (kips/mV/V) -17.3762643

Squid Gain 50
Squid Excitation 5
Force Calibration (kips/V) -3475.25286

Calibrated by: Sean Bonney
Calibrated Date: 1/21/2025


Pile Dynamics Inc
30725 Aurora Rd
Solon, OH 44139

Traceable to N.I.S.T.

Cycle 1
Sample

Force (kips)	Bridge (mV/V)
1 0	0
2 1.09446569	-0.063235618
3 2.01727526	-0.115609762
4 3.01514167	-0.174097114
5 4.10258899	-0.235660064
6 5.1814585	-0.297891266
7 5.94928073	-0.342436948
8 7.12757667	-0.409776829
9 8.30801751	-0.477680743
10 9.14202705	-0.52524056
11 10.0150275	-0.575899695

Serial Number 30399
 Force Calibration (lb/V) -17.4016662
 Offset -0.00374992
 Correlation -0.99999814

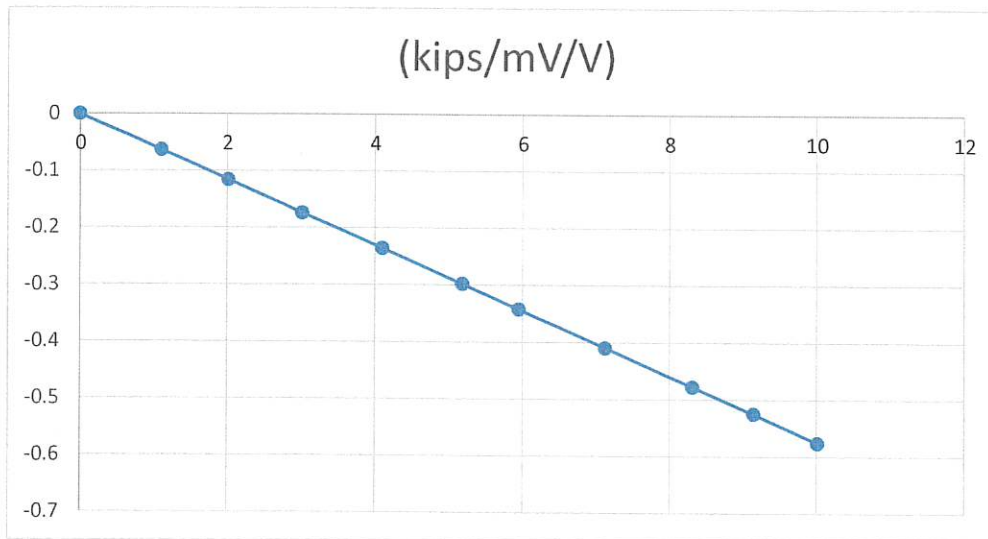


Cycle 2
Sample

Force (kips)	Bridge (mV/V)
1 0	0
2 0.80944452	-0.047208722
3 2.02731531	-0.117401066
4 3.02908078	-0.174571011
5 4.10210159	-0.235205141

6	4.81757884	-0.277447667
7	5.93758358	-0.341233284
8	7.10086819	-0.408227227
9	7.87678139	-0.454076219
10	9.09016969	-0.522994339
11	9.92271741	-0.571956938

Serial Number 30399
 Force Calibration (kips/mV/V) -17.3779217
 Offset -0.00324012
 Correlation -0.9999939

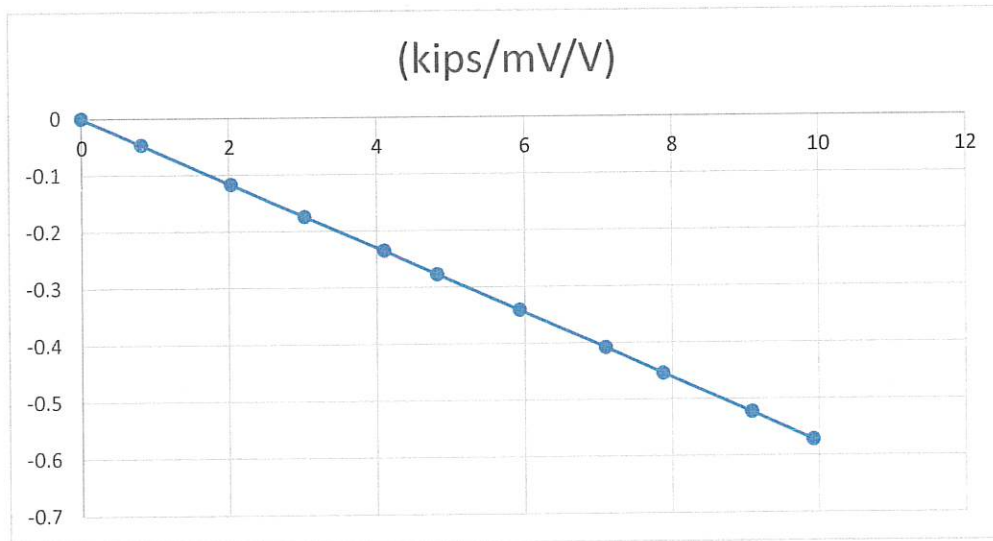

Sample	Cycle 3	
	Force (kips)	Bridge (mV/V)
1	0	0
2	1.13014207	-0.065301771
3	2.01854245	-0.115590808
4	3.03590415	-0.173736961
5	4.07860978	-0.2351767
6	5.18730709	-0.298516805
7	5.96234258	-0.342650204
8	7.13186565	-0.410302854
9	7.92395993	-0.455189847
10	9.19827106	-0.528553076
11	10.1433068	-0.585917804