


Cycle 1
Sample

Force (kips)	Bridge (mV/V)
1 0	0
2 0.82133664	-0.047914818
3 1.95372058	-0.113766347
4 2.88140395	-0.167481642
5 3.89223477	-0.224466821
6 4.85081832	-0.281058728
7 5.78103636	-0.334551453
8 6.89412053	-0.398450883
9 7.80611095	-0.452147516
10 9.0280772	-0.524079597
11 10.0321838	-0.58174762

Serial Number 30409
Force Calibration (lb/V) -17.2566734
Offset 0.00024556
Correlation -0.99999263

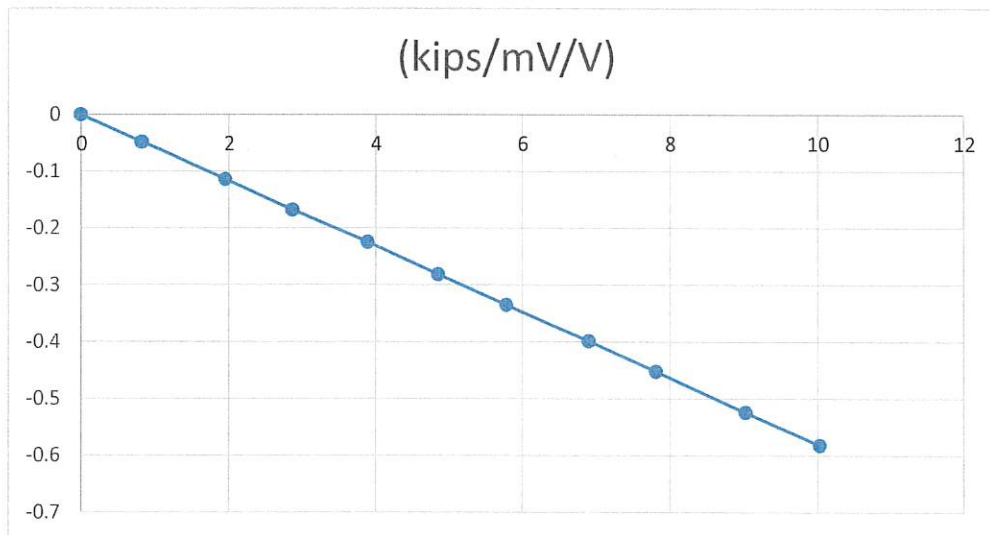


Cycle 2
Sample

Force (kips)	Bridge (mV/V)
1 0	0
2 1.17741816	-0.068040865
3 2.03394374	-0.117837075
4 3.26867792	-0.189162109
5 4.32785708	-0.248867451


6	5.04196966	-0.290967837
7	6.22874581	-0.357355157
8	7.33656631	-0.424036384
9	8.14474426	-0.470634164
10	9.31436562	-0.540992981
11	10.0869652	-0.586899015

Serial Number 30409
 Force Calibration (kips/mV/V) -17.2094001
 Offset 0.02598421
 Correlation -0.99995961

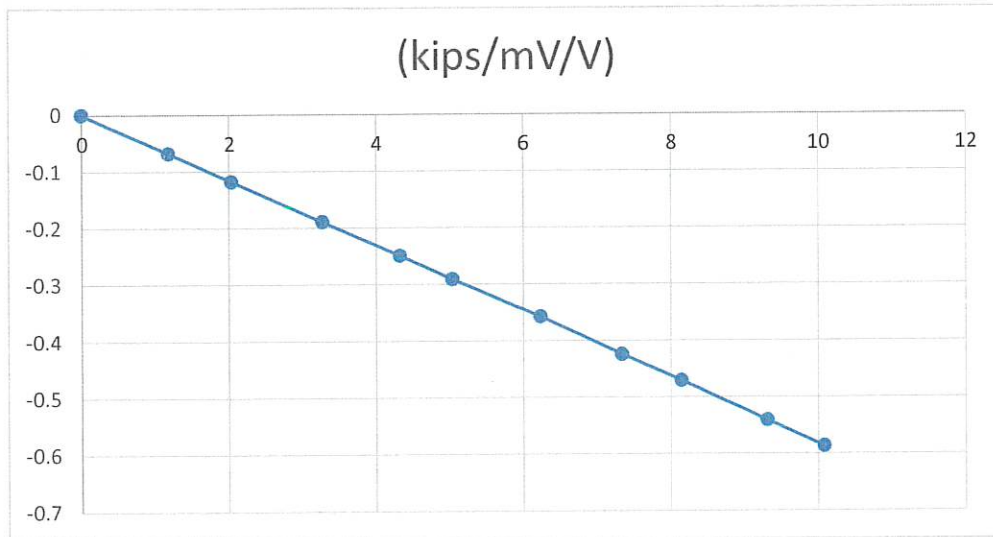

Sample	Cycle 3	
	Force (kips)	Bridge (mV/V)
1	0	0
2	1.13979224	-0.064875294
3	2.01552068	-0.114486688
4	3.21457848	-0.182451848
5	4.21312729	-0.240991418
6	4.94527301	-0.282271971
7	6.03847172	-0.345706945
8	7.15145844	-0.409108832
9	7.94394263	-0.455474393
10	9.18247988	-0.525596243
11	9.97321011	-0.572639608

Serial Number 30409
Force Calibration (kips/mV/V) -17.4009268
Offset 0.02461984
Correlation -0.99999366

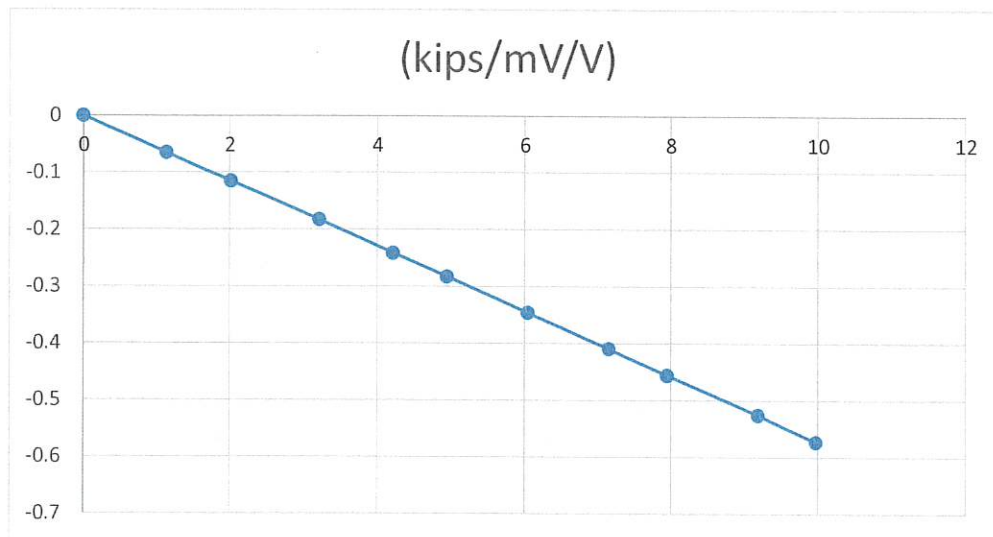

Serial Number 30409
Force Calibration (kips/mV/V) -17.2890001

Squid Gain 50
Squid Excitation 5
Force Calibration (kips/V) -3457.80002

Calibrated by: Sean Benson
Calibrated Date: 1/21/2025

Pile Dynamics Inc
30725 Aurora Rd
Solon, OH 44139

Traceable to N.I.S.T.

