


Cycle 1
Sample

	Force (kips)	Bridge (mV/V)
1	0	0
2	1.14447111	-0.06366685
3	2.04915005	-0.114917873
4	3.08337518	-0.172732294
5	4.17228465	-0.233484883
6	5.25641791	-0.294517132
7	6.0468547	-0.337669566
8	7.20175632	-0.40347876
9	8.00730239	-0.447991362
10	9.27547255	-0.518795544
11	10.113674	-0.57219376

Serial Number 30500DC
Force Calibration (lb/V) -17.7638753
Offset 0.02267181
Correlation -0.9999482

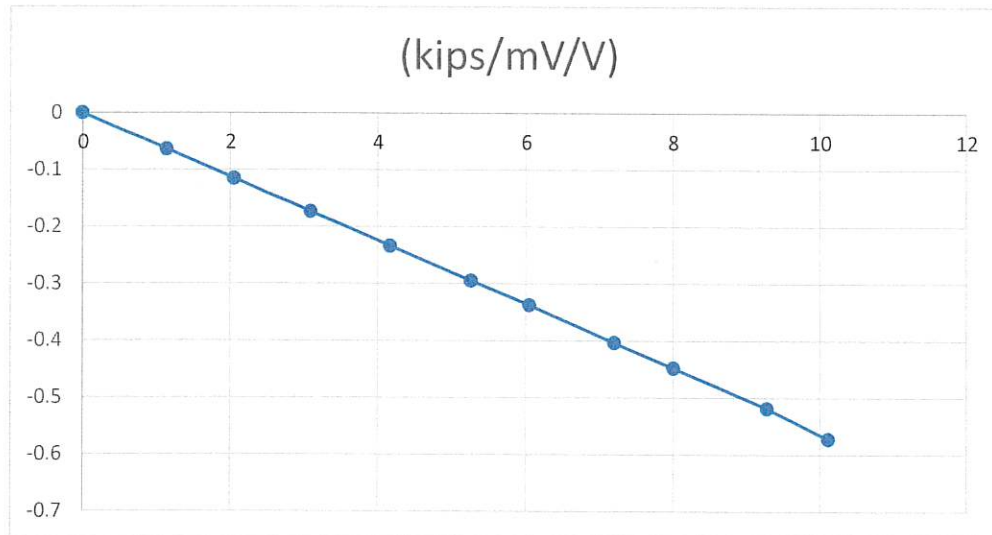


Cycle 2
Sample

	Force (kips)	Bridge (mV/V)
1	0	0
2	1.12049189	-0.062557954
3	2.01210899	-0.112264102
4	3.05491204	-0.170296513
5	4.11136186	-0.230034979


6	4.85744671	-0.270926909
7	5.99831143	-0.335522859
8	7.1700765	-0.400550134
9	7.97737715	-0.446583928
10	9.01706221	-0.503754234
11	9.81997699	-0.548333291

Serial Number 30500DC
 Force Calibration (kips/mV/V) -17.8890597
 Offset 0.00260652
 Correlation -0.99999707

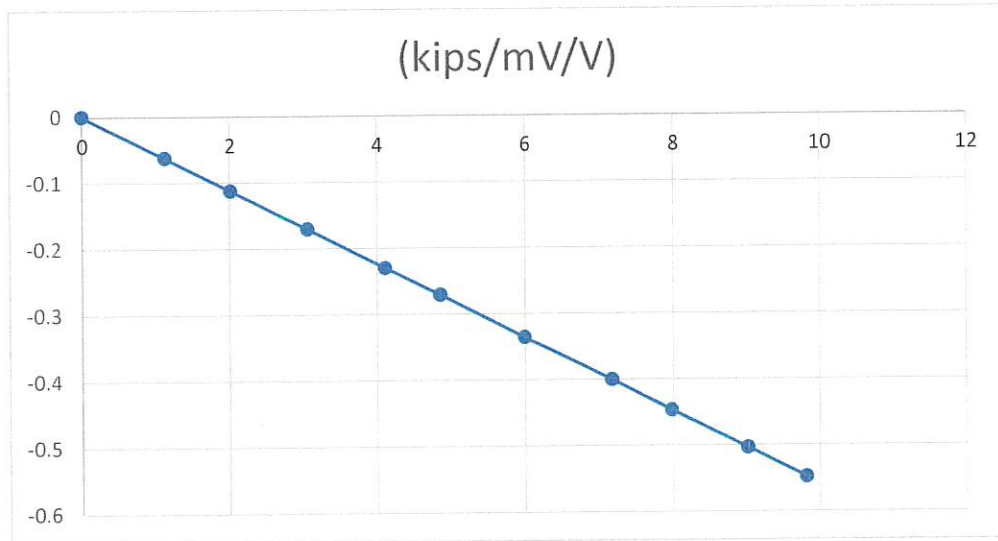

Sample	Cycle 3	
	Force (kips)	Bridge (mV/V)
1	0	0
2	0.85993732	-0.047744212
3	2.04612826	-0.11427813
4	2.90957465	-0.162297271
5	3.97723425	-0.222215809
6	5.0899281	-0.284129485
7	5.84069196	-0.326376784
8	7.02561633	-0.391683644
9	7.82092735	-0.436750692
10	9.01803705	-0.502512649
11	10.0234108	-0.559010108

Serial Number 30500DC
Force Calibration (kips/mV/V) -17.9324316
Offset -0.00286112
Correlation -0.99999792

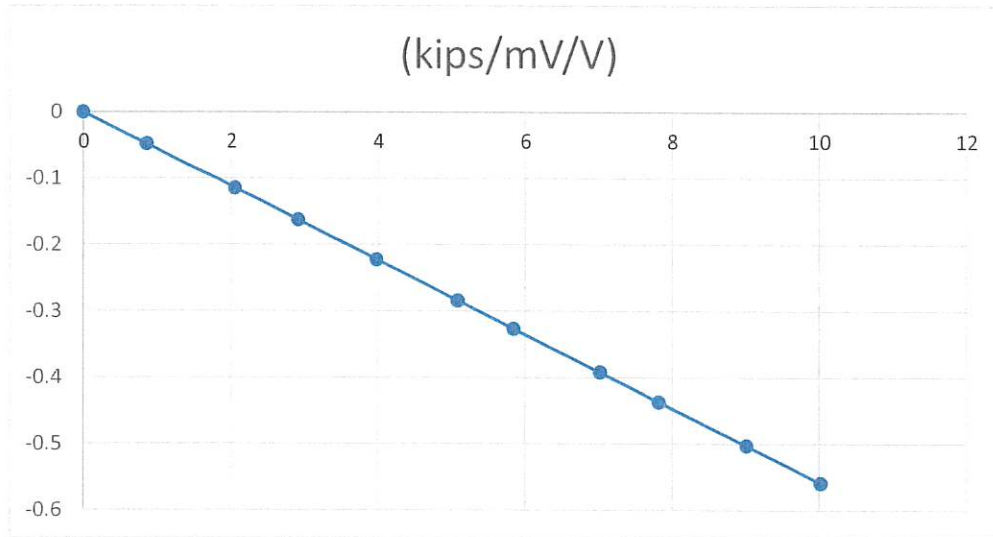

Serial Number 30500DC
Force Calibration (kips/mV/V) -17.8617889
Squid Gain 50
Squid Excitation 5
Force Calibration (kips/V) -3572.35778

Calibrated by: Sean Bonney
Calibrated Date: 3/24/2025

Pile Dynamics Inc
30725 Aurora Rd
Solon, OH 44139

Traceable to N.I.S.T.

