


6	5.17112599	-0.296389035
7	5.93680375	-0.339868462
8	7.11188299	-0.407307856
9	7.88448196	-0.452782471
10	8.86519363	-0.508715934
11	9.86900765	-0.567383837

Serial Number 30502DC
 Force Calibration (kips/mV/V) -17.3903439
 Offset 0.01602268
 Correlation -0.99999601

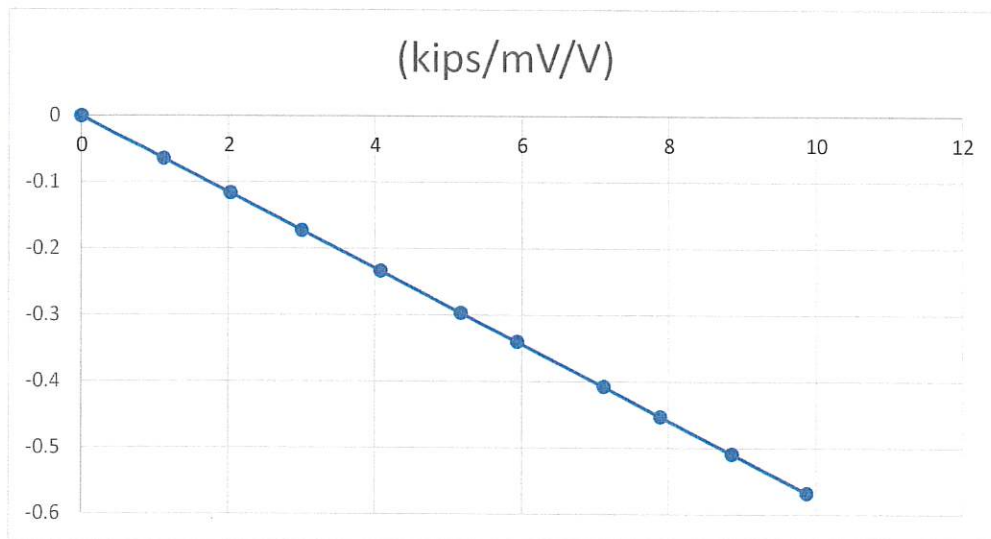


Sample	Cycle 3	
	Force (kips)	Bridge (mV/V)
1	0	0
2	1.13433357	-0.063827974
3	2.0047008	-0.113249789
4	3.3109827	-0.186844714
5	4.02626492	-0.227475974
6	5.10542685	-0.289403871
7	6.30545981	-0.358061086
8	7.09453212	-0.403796284
9	8.28033414	-0.471667007
10	9.07125901	-0.516923693
11	10.2465345	-0.584358622

Cycle 1
Sample

Force (kips)	Bridge (mV/V)
1 0	0
2 0.85477107	-0.049544991
3 2.08658099	-0.120509776
4 3.11534744	-0.179480503
5 3.84310664	-0.220746776
6 4.90384552	-0.282333475
7 6.11733024	-0.351540406
8 6.88515266	-0.396346782
9 7.79646073	-0.448417959
10 9.00663228	-0.517321854
11 9.89025773	-0.573591877


Serial Number 30502DC
 Force Calibration (lb/V) -17.3294754
 Offset 0.00878024
 Correlation -0.99996608

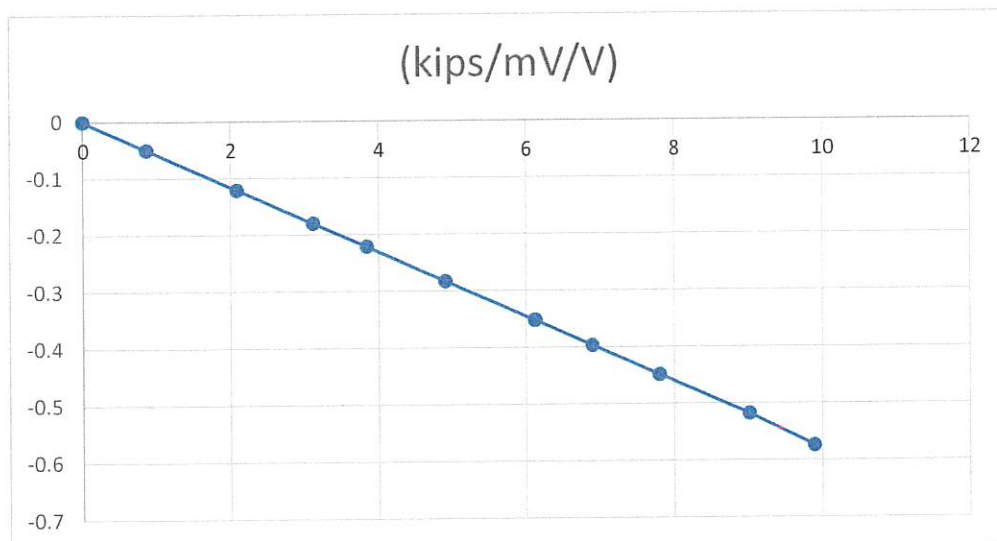

Cycle 2
Sample

Force (kips)	Bridge (mV/V)
1 0	0
2 1.12117423	-0.064112311
3 2.02751027	-0.11583249
4 3.00861074	-0.17198357
5 4.07841482	-0.233352222

Serial Number 30502DC
Force Calibration (kips/mV/V) -17.4910666
Offset 0.03353968
Correlation -0.99999471

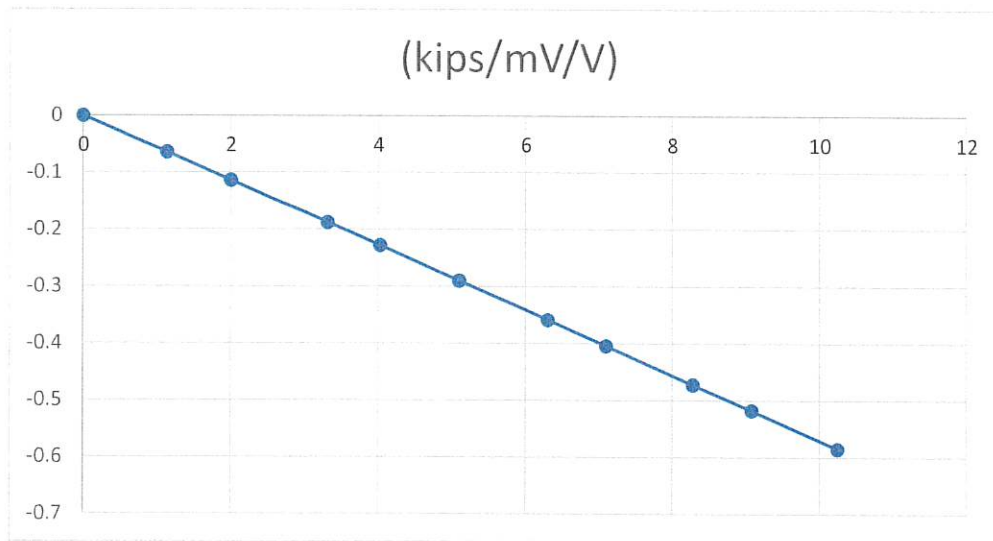

Serial Number 30502DC
Force Calibration (kips/mV/V) -17.4036287

Squid Gain 50
Squid Excitation 5
Force Calibration (kips/V) -3480.72573

Calibrated by: Sean Bourke
Calibrated Date: 3/20/2025

Pile Dynamics Inc
30725 Aurora Rd
Solon, OH 44139

Traceable to N.I.S.T.

