


6	5.23000178	-0.303237034
7	6.00221047	-0.347692736
8	7.15428527	-0.414274485
9	8.00506044	-0.464322231
10	9.22917119	-0.536022219
11	9.8879181	-0.575469118

Serial Number 30504DC
 Force Calibration (kips/mV/V) -17.1986175
 Offset 0.0122907
 Correlation -0.9999937

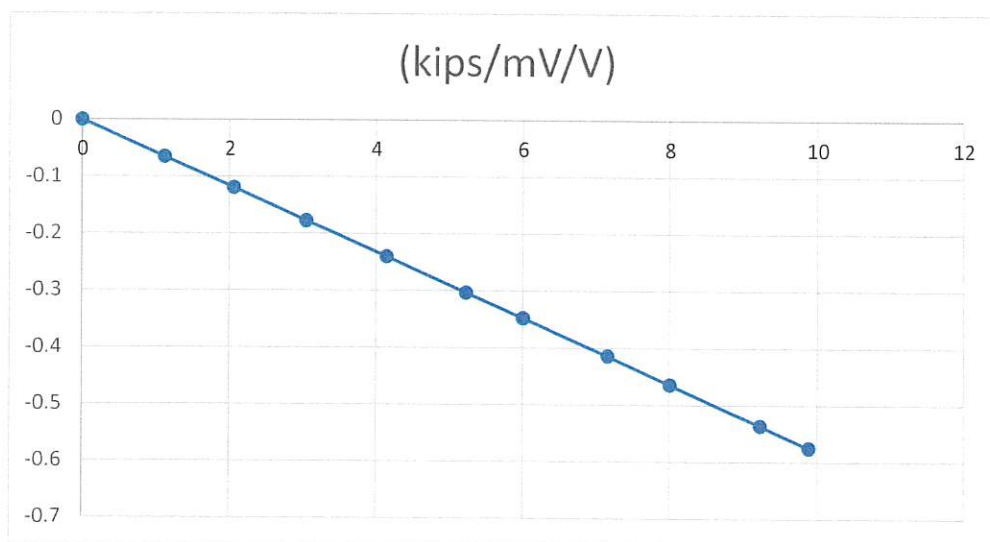


Sample	Cycle 3	
	Force (kips)	Bridge (mV/V)
1	0	0
2	0.8401496	-0.048090198
3	2.08043997	-0.119277781
4	3.10150578	-0.178765113
5	3.82058958	-0.218789844
6	4.92694744	-0.283371609
7	6.05182604	-0.348228319
8	6.842263	-0.39333805
9	8.04619564	-0.462554737
10	8.82103687	-0.508541297
11	9.94923109	-0.574469368

Cycle 1
Sample

Force (kips)	Bridge (mV/V)
1 0	0
2 0.84297642	-0.049350736
3 1.98773986	-0.115932111
4 2.96230941	-0.172391277
5 4.01417782	-0.233944818
6 4.77205733	-0.277424247
7 5.90765831	-0.342788001
8 7.0714303	-0.410739299
9 7.87171264	-0.456796874
10 9.04698762	-0.525790929
11 9.84941506	-0.575369674


Serial Number 30504DC
 Force Calibration (lb/V) -17.1842426
 Offset 0.00151853
 Correlation -0.99998431

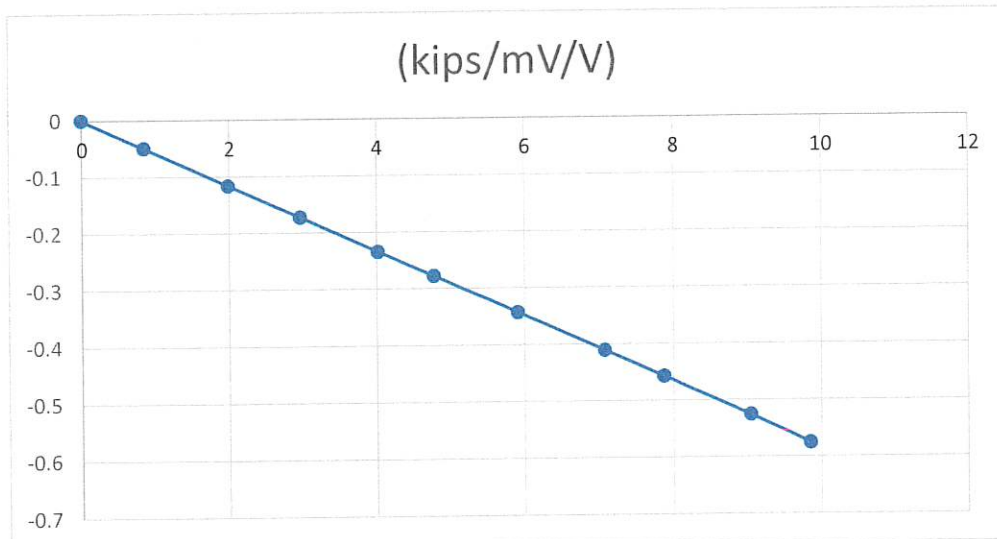

Cycle 2
Sample

Force (kips)	Bridge (mV/V)
1 0	0
2 1.12945973	-0.065325515
3 2.05899517	-0.119310929
4 3.05812878	-0.177376578
5 4.14089723	-0.239858941

Serial Number 30504DC
Force Calibration (kips/mV/V) -17.3261633
Offset 0.01552765
Correlation -0.9999924

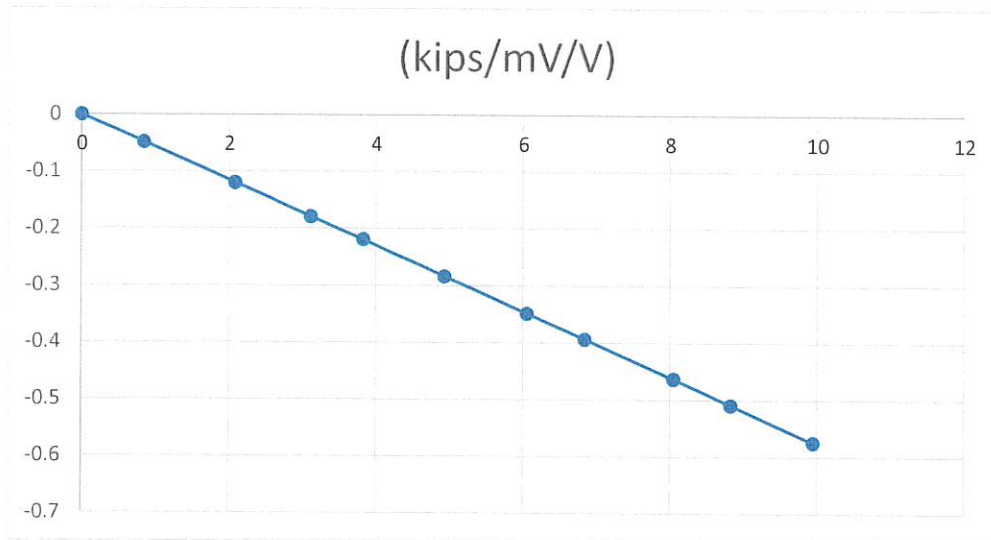

Serial Number 30504DC
Force Calibration (kips/mV/V) -17.2363412

Squid Gain 50
Squid Excitation 5
Force Calibration (kips/V) -3447.26823

Calibrated by: Sean Bonny
Calibrated Date: 3/24/2025

Pile Dynamics Inc
30725 Aurora Rd
Solon, OH 44139

Traceable to N.I.S.T.

