


Cycle 1
Sample

Force (kips)	Bridge (mV/V)
1 0	0
2 1.0451426	-0.061335321
3 1.98033168	-0.112586343
4 2.96718325	-0.16598412
5 3.99273302	-0.224447818
6 5.05815076	-0.284328505
7 6.17942272	-0.347578621
8 6.96352371	-0.391536718
9 8.12836825	-0.456763104
10 9.2797615	-0.520676909
11 9.97126057	-0.562455276

Serial Number 30505DC
 Force Calibration (lb/V) -17.8233364
 Offset -0.01800416
 Correlation -0.99997946

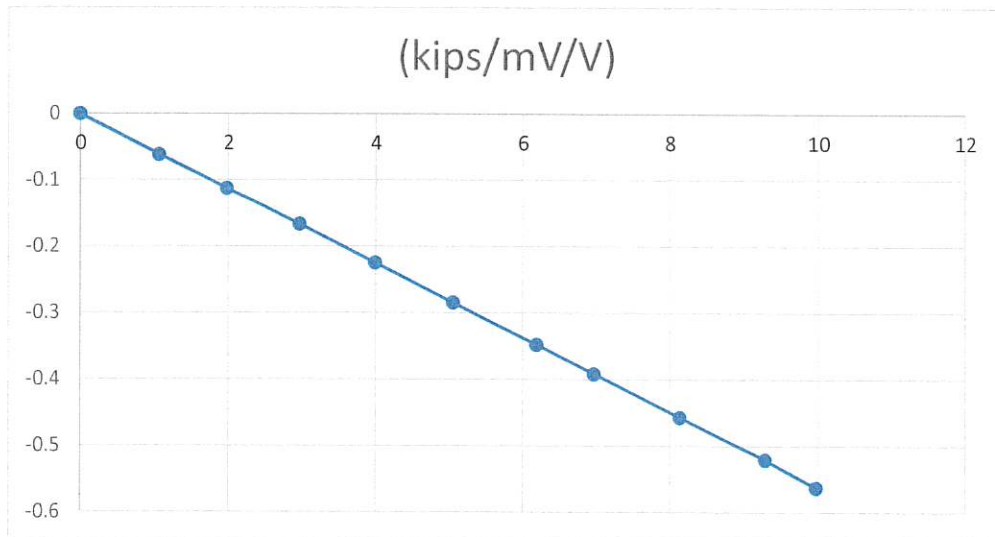


Cycle 2
Sample

Force (kips)	Bridge (mV/V)
1 0	0
2 0.81305114	-0.045398471
3 2.02409857	-0.11259584
4 3.007441	-0.167277866
5 4.05843214	-0.226423978


6	4.78706871	-0.267197442
7	5.91740597	-0.330750842
8	6.70267666	-0.375149654
9	7.89422975	-0.440461336
10	8.70981615	-0.486215588
11	9.84210439	-0.557669095

Serial Number 30505DC
 Force Calibration (kips/mV/V) -17.7471047
 Offset 0.03527997
 Correlation -0.99991652

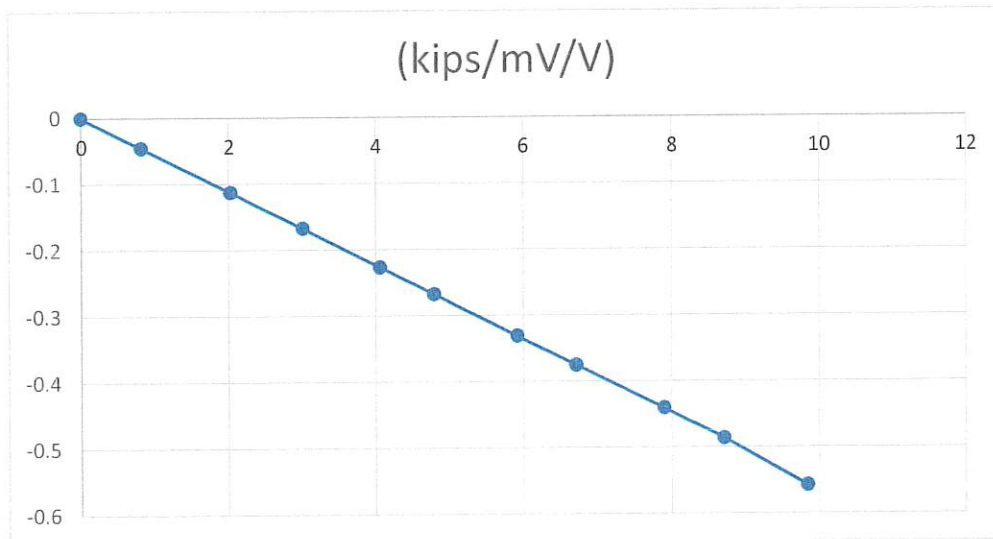

Sample	Cycle 3	
	Force (kips)	Bridge (mV/V)
1	0	0
2	1.06220098	-0.059989479
3	2.0485652	-0.115235381
4	3.01982054	-0.169467204
5	4.07646529	-0.228973463
6	5.15455499	-0.289806674
7	6.33353306	-0.35508031
8	7.10418231	-0.398720908
9	8.30138911	-0.465530104
10	9.02797946	-0.506483842
11	10.079947	-0.564857919

Serial Number 30505DC
Force Calibration (kips/mV/V) -17.8514697
Offset -0.00974912
Correlation -0.99999884

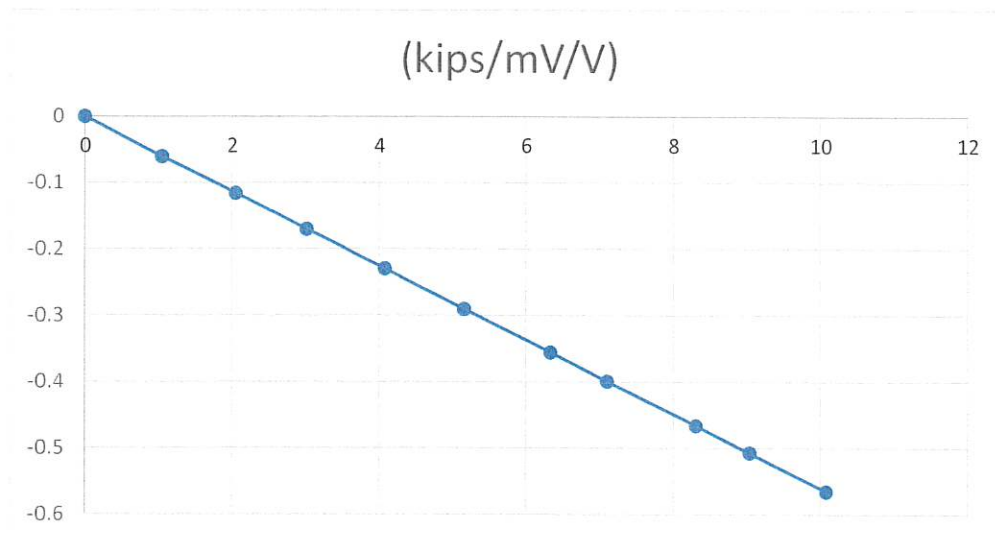

Serial Number 30505DC
Force Calibration (kips/mV/V) -17.8073036
Squid Gain 50
Squid Excitation 5
Force Calibration (kips/V) -3561.46072

Calibrated by: Sam Bonner
Calibrated Date: 3/24/2025

Pile Dynamics Inc
30725 Aurora Rd
Solon, OH 44139

Traceable to N.I.S.T.

