


Cycle 1
Sample

	Force (kips)	Bridge (mV/V)
1	0	0
2	1.11766509	-0.064079138
3	2.06854787	-0.11922079
4	3.08201052	-0.176992572
5	4.16770326	-0.239327962
6	5.24803493	-0.302151529
7	6.01078839	-0.345441404
8	7.19210612	-0.413913886
9	7.96295052	-0.458573411
10	8.98187301	-0.51789521
11	10.2221654	-0.588055032

Serial Number 30508DC
Force Calibration (lb/V) -17.3579725
Offset 0.0063085
Correlation -0.99999712

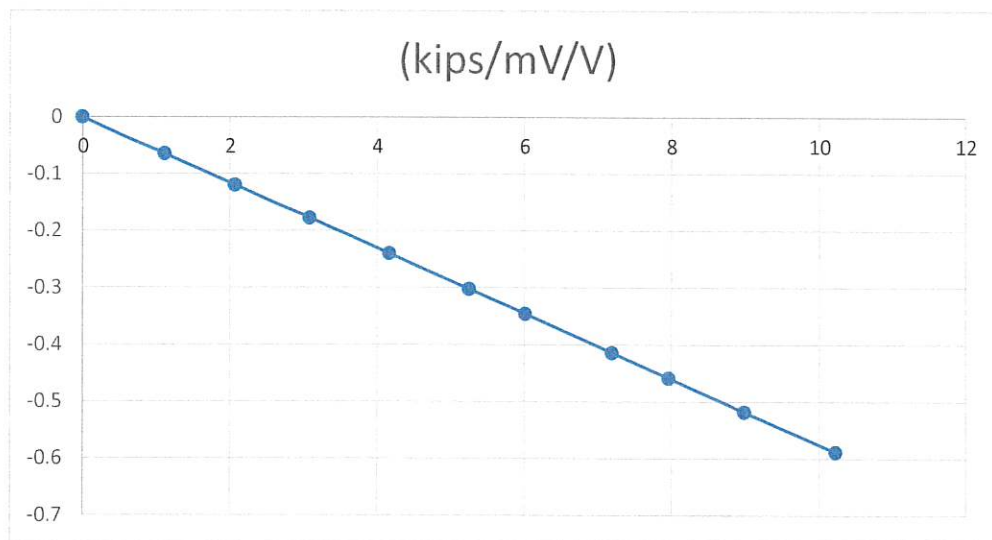


Cycle 2
Sample

	Force (kips)	Bridge (mV/V)
1	0	0
2	1.00108324	-0.057714821
3	2.07576111	-0.119149711
4	2.89583048	-0.166358509
5	3.95208533	-0.227106362


6	5.07647634	-0.291389498
7	5.96487698	-0.342763936
8	7.12075336	-0.409260292
9	7.93312277	-0.456677864
10	8.92884585	-0.513630202
11	10.2110532	-0.589339311

Serial Number 30508DC
 Force Calibration (kips/mV/V) -17.3450163
 Offset 0.01173787
 Correlation -0.99999395

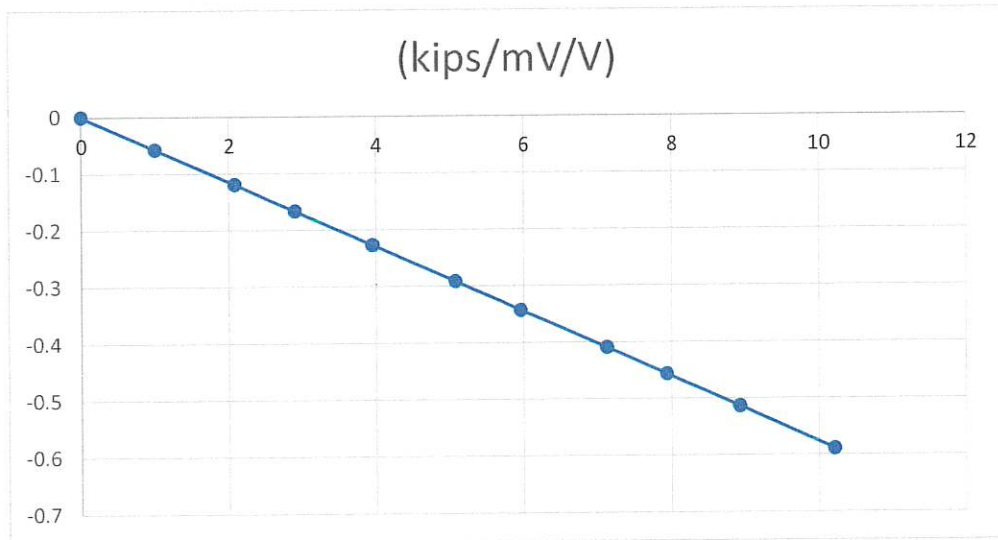

Sample	Cycle 3	
	Force (kips)	Bridge (mV/V)
1	0	0
2	1.02486748	-0.058278761
3	2.03833014	-0.117557473
4	2.91464342	-0.167870257
5	3.95666671	-0.227599267
6	4.84750412	-0.278973659
7	5.80560043	-0.334371434
8	6.7942071	-0.391309418
9	7.83096746	-0.450555327
10	8.85027988	-0.510142524
11	9.81149667	-0.566208784

Serial Number 30508DC
Force Calibration (kips/mV/V) -17.3300567
Offset 0.01017041
Correlation -0.99999725

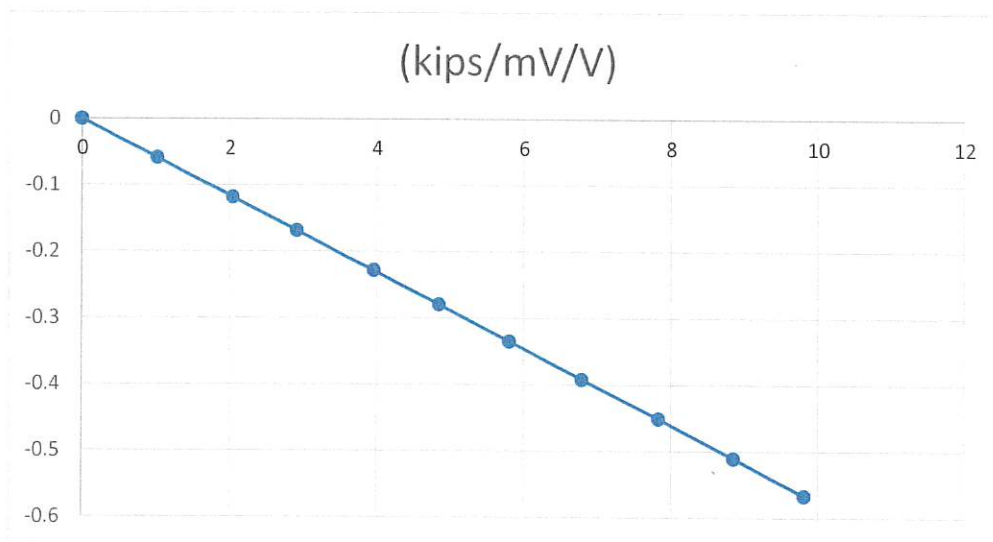

Serial Number 30508DC
Force Calibration (kips/mV/V) -17.3443485

Squid Gain 50
Squid Excitation 5
Force Calibration (kips/V) -3468.86969

Calibrated by: Sean Donnan
Calibrated Date: 3/24/2025

Pile Dynamics Inc
30725 Aurora Rd
Solon, OH 44139

Traceable to N.I.S.T.

