


Cycle 1
Sample

Force (kips)	Bridge (mV/V)
1 0	0
2 0.91891059	-0.05080553
3 1.90966124	-0.106331022
4 2.9276078	-0.163865846
5 4.01125354	-0.224495221
6 5.10006565	-0.285366343
7 5.87149451	-0.328613553
8 7.04569645	-0.393858812
9 8.22106851	-0.460009298
10 9.05147141	-0.50634171
11 10.2442927	-0.574411642

Serial Number 30511DC
 Force Calibration (lb/V) -17.8383712
 Offset 0.01078363
 Correlation -0.99999766

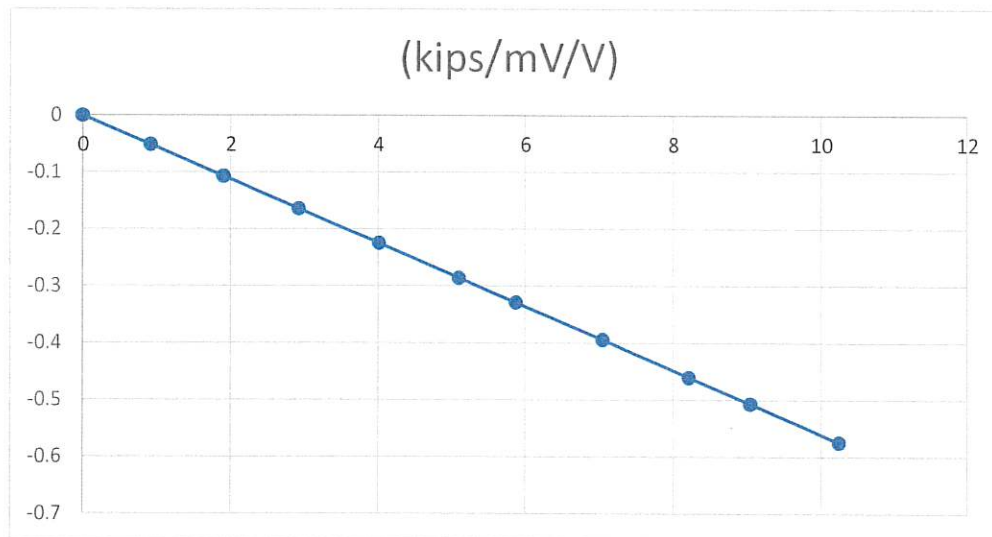


Cycle 2
Sample

Force (kips)	Bridge (mV/V)
1 0	0
2 0.89795314	-0.050525938
3 1.83470183	-0.102743691
4 2.77846882	-0.155326378
5 3.77428826	-0.211122077


6	4.79145515	-0.267827697
7	5.91565139	-0.330741341
8	7.09375244	-0.397318243
9	7.88721143	-0.44147543
10	9.07973979	-0.508019325
11	10.03735	-0.561531275

Serial Number	30511DC
Force Calibration (kips/mV/V)	-17.8739142
Offset	-0.00071775
Correlation	-0.99999919

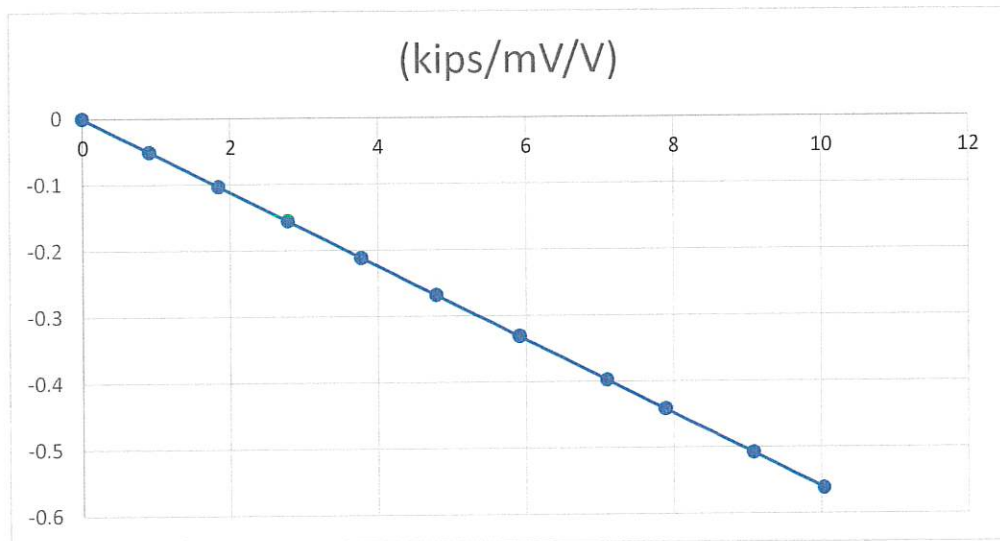

Sample	Cycle 3	
	Force (kips)	Bridge (mV/V)
1	0	0
2	0.93470178	-0.052051851
3	2.19273286	-0.121964593
4	3.16067401	-0.17675087
5	4.22960081	-0.235617382
6	4.93766984	-0.276315019
7	6.08087399	-0.339223921
8	7.12816155	-0.399554936
9	7.97649979	-0.443996449
10	8.90291704	-0.502427299
11	10.0218509	-0.561834451

Serial Number 30511DC
Force Calibration (kips/mV/V) -17.7939437
Offset 0.02312016
Correlation -0.99995388

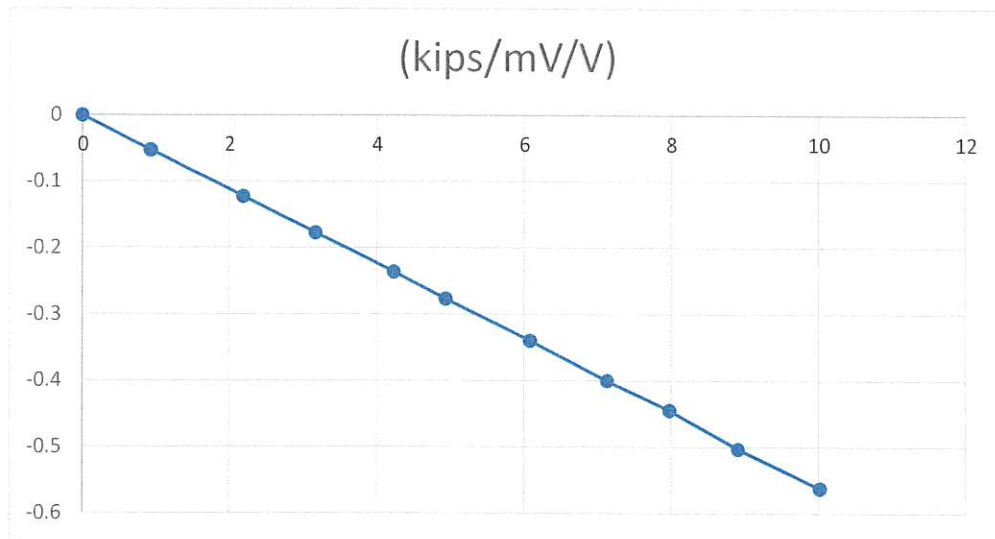

Serial Number 30511DC
Force Calibration (kips/mV/V) -17.8354097

Squid Gain 50
Squid Excitation 5
Force Calibration (kips/V) -3567.08194

Calibrated by: Sean Barry
Calibrated Date: 3/20/2025

Pile Dynamics Inc
30725 Aurora Rd
Solon, OH 44139

Traceable to N.I.S.T.

