


Cycle 1
Sample

	Force (kips)	Bridge (mV/V)
1	0	0
2	0.89288436	-0.051123049
3	1.92126093	-0.110667133
4	2.77973602	-0.160107956
5	3.83511357	-0.220723132
6	4.93961938	-0.284755121
7	6.08145889	-0.350218341
8	6.86439017	-0.395176375
9	8.05574835	-0.465236504
10	8.86568115	-0.509450648
11	9.75018384	-0.566431522

Serial Number 30512DC
Force Calibration (lb/V) -17.282733
Offset 0.01695511
Correlation -0.99996536

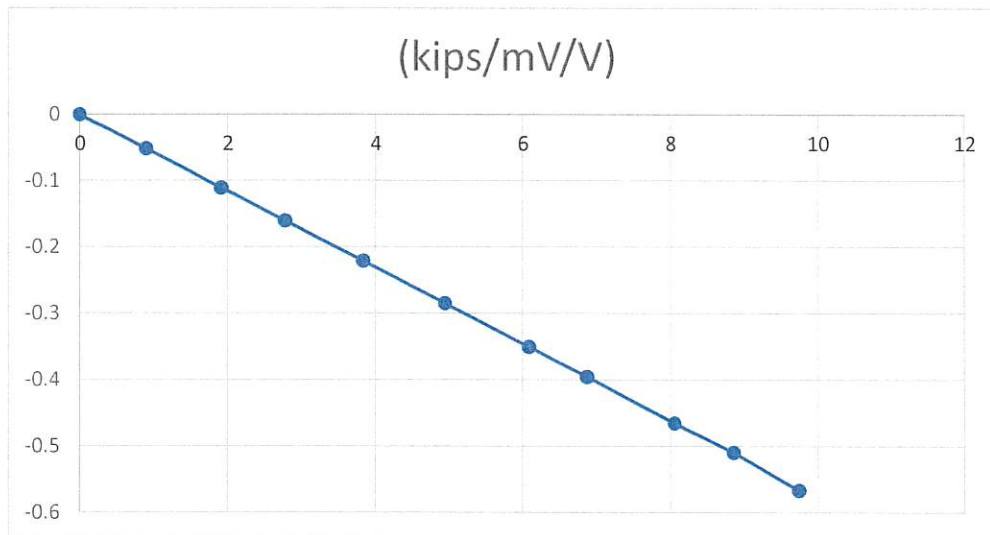


Cycle 2
Sample

	Force (kips)	Bridge (mV/V)
1	0	0
2	1.06493032	-0.061425373
3	2.23289316	-0.12815835
4	2.97771071	-0.171263282
5	4.06262363	-0.233646068


6	5.08154511	-0.291920297
7	5.99567954	-0.344612161
8	6.99442377	-0.401905566
9	8.03167152	-0.46198079
10	9.23794406	-0.532031538
11	9.87212686	-0.568876709

Serial Number 30512DC
 Force Calibration (kips/mV/V) -17.3604825
 Offset 0.00705692
 Correlation -0.99999735

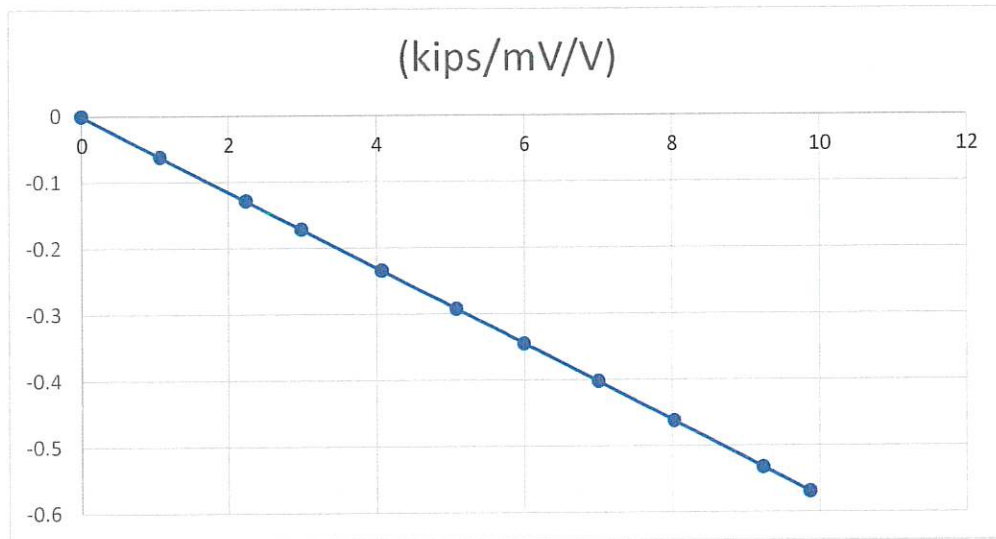

Sample	Cycle 3	
	Force (kips)	Bridge (mV/V)
1	0	0
2	1.17780806	-0.067965028
3	2.12937318	-0.122286864
4	3.14147116	-0.181110689
5	4.23720398	-0.243337099
6	5.33050002	-0.306667743
7	6.11382103	-0.350834327
8	7.28753562	-0.419259441
9	8.07290404	-0.464516084
10	9.16542139	-0.527648
11	9.94728122	-0.572738902

Serial Number 30512DC
Force Calibration (kips/mV/V) -17.3724385
Offset 0.00323332
Correlation -0.99999719

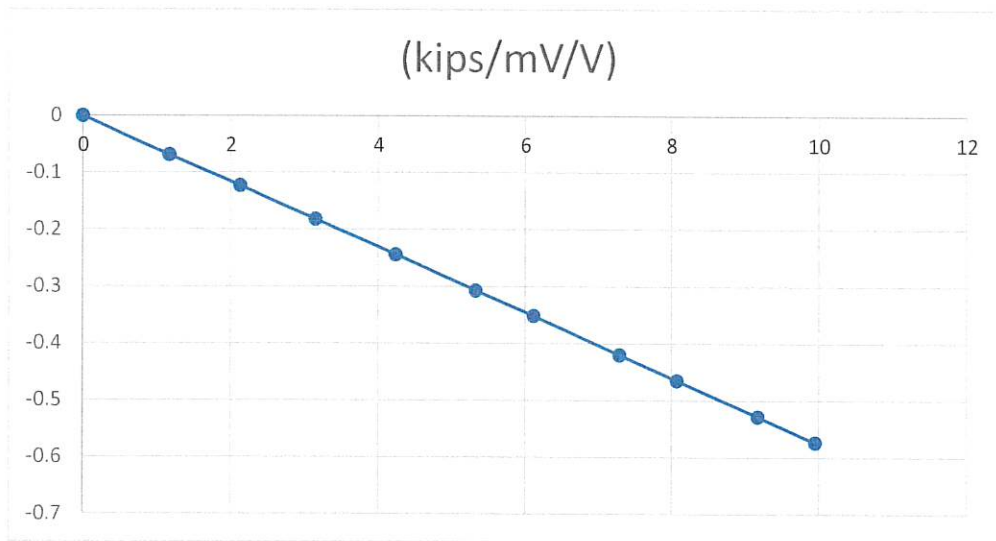

Serial Number 30512DC
Force Calibration (kips/mV/V) -17.3385513
Squid Gain 50
Squid Excitation 5
Force Calibration (kips/V) -3467.71027

Calibrated by: Joan Benson
Calibrated Date: 3/20/2025

Pile Dynamics Inc
30725 Aurora Rd
Solon, OH 44139

Traceable to N.I.S.T.

