


Cycle 1
Sample

	Force (kips)	Bridge (mV/V)
1	0	0
2	0.92446674	-0.050995082
3	2.10510152	-0.118173489
4	2.84640992	-0.159340198
5	3.91134017	-0.218130873
6	4.91710231	-0.275409899
7	5.8512194	-0.327433543
8	6.88544506	-0.384347794
9	7.97308818	-0.445617177
10	8.97037091	-0.502986514
11	9.94884107	-0.557564704

Serial Number 3052DC
Force Calibration (lb/V) -17.8408634
Offset 0.00971734
Correlation -0.99999316

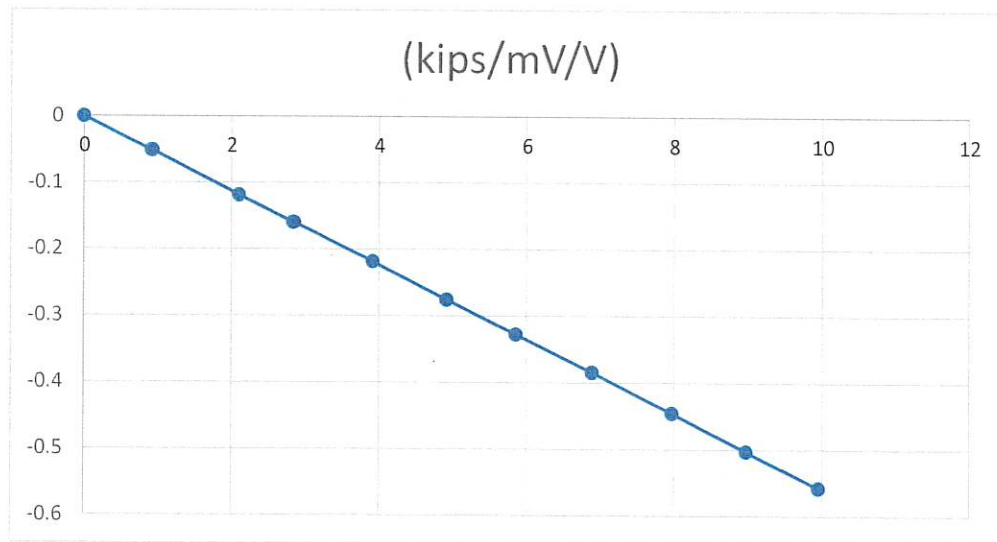


Cycle 2
Sample

	Force (kips)	Bridge (mV/V)
1	0	0
2	0.82884233	-0.047374584
3	1.77514372	-0.100317387
4	2.80147326	-0.157349891
5	3.78842235	-0.212306811


6	4.95170647	-0.276736842
7	5.89098984	-0.330025786
8	6.7522922	-0.378628008
9	7.70726973	-0.431670644
10	8.70221297	-0.487073326
11	9.80720772	-0.549413874

Serial Number 3052DC
 Force Calibration (kips/mV/V) -17.8871554
 Offset -0.01353386
 Correlation -0.99999746

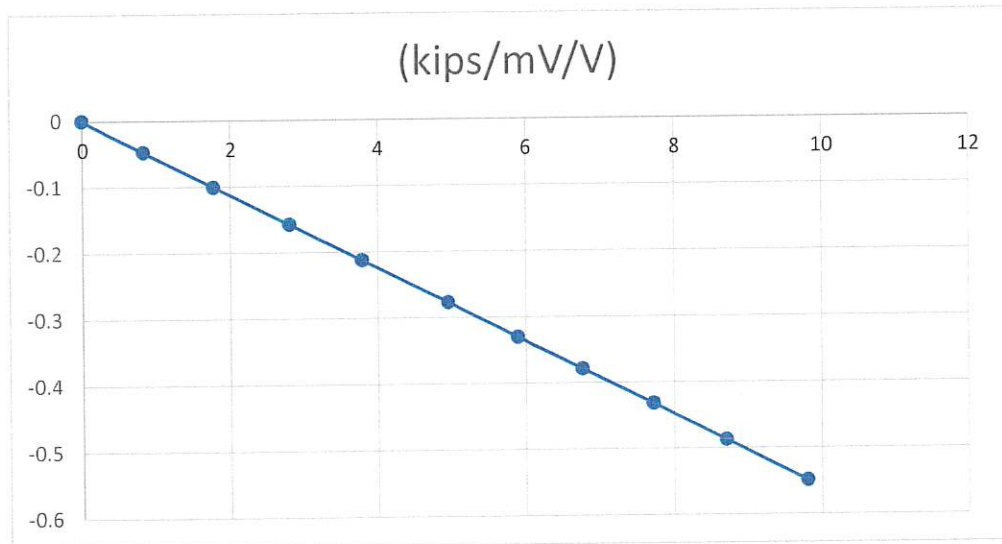

Sample	Cycle 3	
	Force (kips)	Bridge (mV/V)
1	0	0
2	1.04017131	-0.058733794
3	2.16524451	-0.122912638
4	3.11593232	-0.175869837
5	4.29188827	-0.242304544
6	5.02881034	-0.284262857
7	6.06293831	-0.342693688
8	7.20994432	-0.408432027
9	8.09834544	-0.461773425
10	9.36456607	-0.529255902
11	10.3248082	-0.586767758

Serial Number 3052DC
Force Calibration (kips/mV/V) -17.6000381
Offset 0.01536129
Correlation -0.99997519

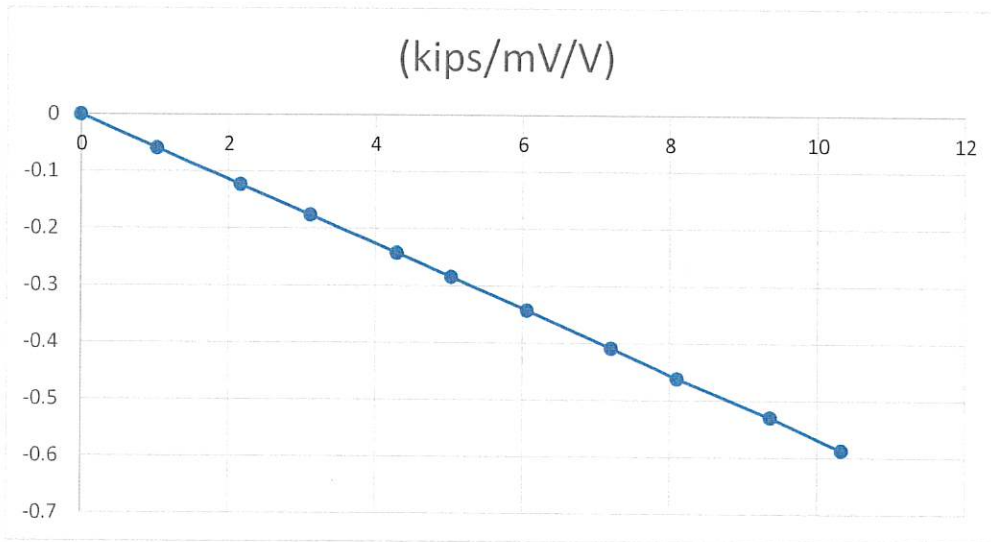

Serial Number 3052DC
Force Calibration (kips/mV/V) -17.776019

Squid Gain 50
Squid Excitation 5
Force Calibration (kips/V) -3555.2038

Calibrated by: Jean Bonney
Calibrated Date: 7/14/2025

Pile Dynamics Inc
30725 Aurora Rd
Solon, OH 44139

Traceable to N.I.S.T.

