


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

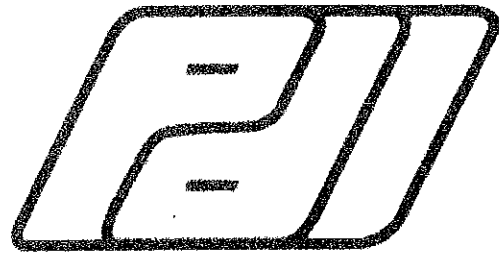

Serial No: 33424 Temperature: 22.3 °C

Model: PE Humidity: 28%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

1217.3 g's/volt

R²: 0.999919 [No chip]

Ref Acc 1: 78268! Cal on: 11Jan2024
986 g's/volt

Ref Acc 2: 78270! Cal on: 11Jan2024
971 g's/volt


Operator: William Johnson

Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: 14Nov2025

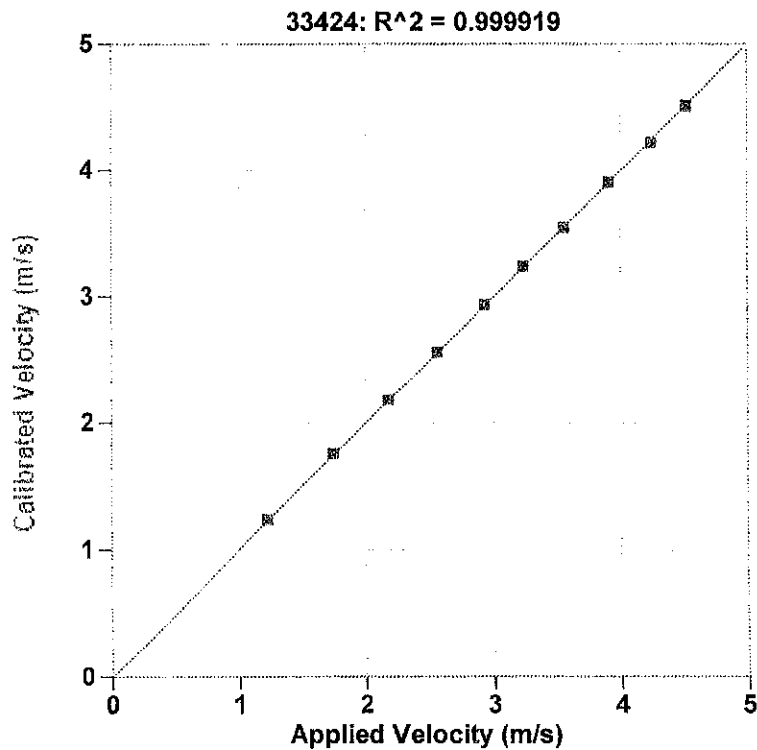

Reference Velocity	S/N 33424 Velocity
m/s	m/s
1.233	1.243
1.752	1.759
2.185	2.190
2.563	2.568
2.933	2.945
3.242	3.249
3.562	3.559
3.914	3.916
4.248	4.228
4.521	4.517
Maximum Acceleration: 981 g's	