


Certificate of Calibration

Pile Dynamics, Inc.

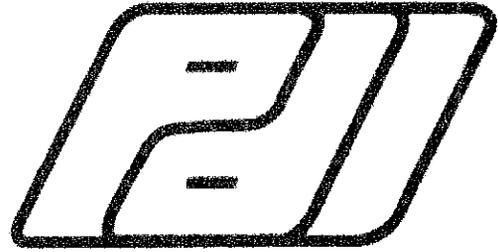

Calibrated by Pile Dynamics, Inc.

Serial No: 72320 Temperature: 20.1 °C
 Model: PE Humidity: 26%
 Calibrated on: Channel 4 on 8G 5028 LE

PDA CALIBRATION FACTOR
 1096.2 g's/volt
 R²: 0.999930 [Chip programmed]

Ref Acc 1: 78268! Cal on: 11Jan2024
 986 g's/volt
 Ref Acc 2: 78270! Cal on: 11Jan2024
 971 g's/volt


Operator: William Johnson

Signed

Calibration valid 2 years

From: 02Jan2026

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

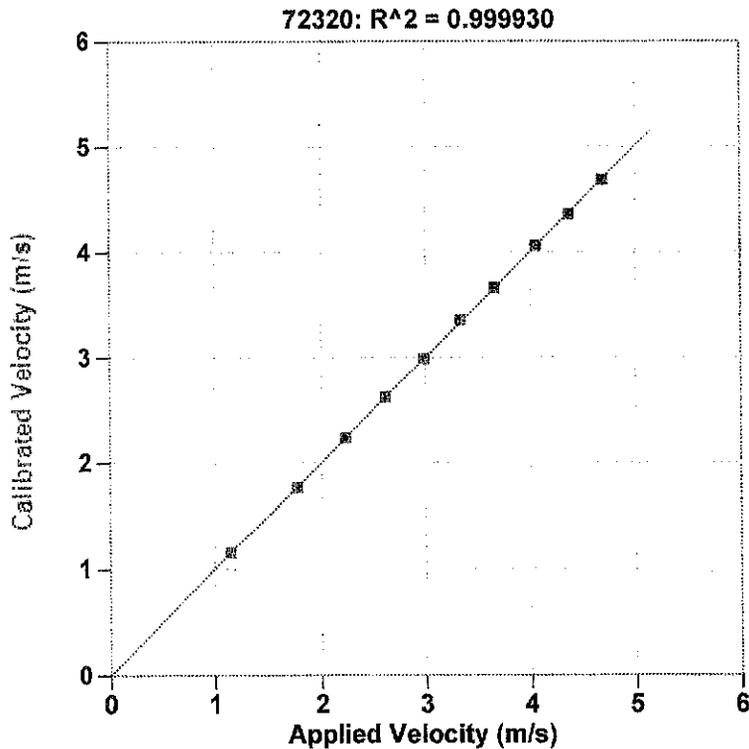

Reference Velocity	S/N 72320 Velocity
m/s	m/s
1.160	1.154
1.774	1.770
2.243	2.239
2.624	2.625
2.990	2.995
3.337	3.358
3.665	3.663
4.059	4.067
4.376	4.366
4.700	4.689

Maximum Acceleration: 1024 g's