




Pile Dynamics, Inc.

Transducer C027

Strain ($\mu\epsilon$)

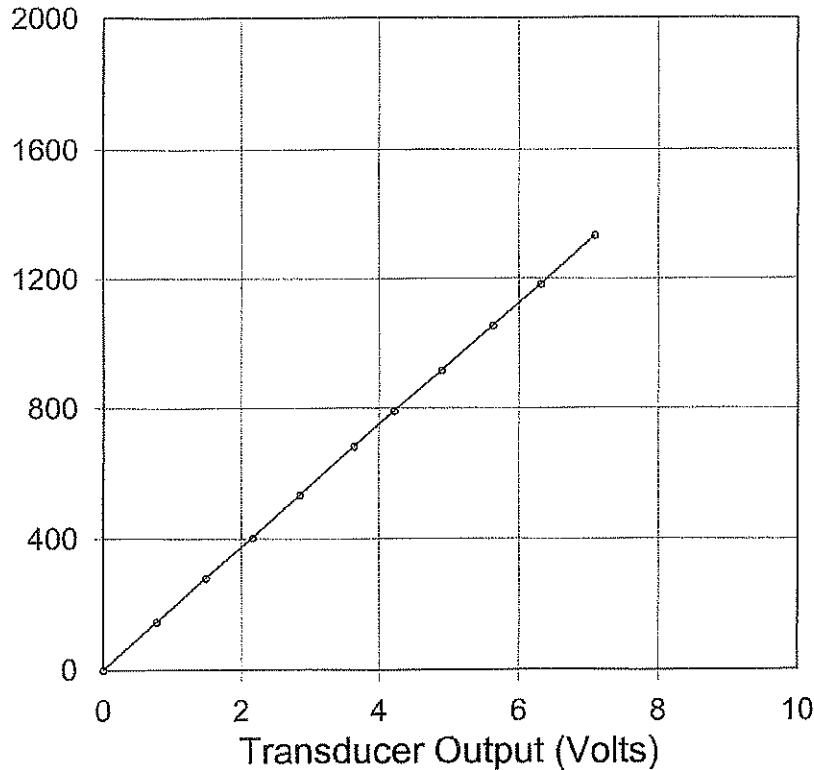

PDA Cal Factor (5.0 V)

93.7 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
148	0.76
282	1.47
404	2.16
533	2.85
683	3.63
792	4.21
916	4.89
1055	5.62
1182	6.31
1334	7.09

Shunt (60.4 K Ω)

2.5 V

General Factor

325.4 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

Calibrated by: 

Calibrated on:

04-Jan-2008