




Pile Dynamics, Inc.

Transducer C029

Strain ($\mu\epsilon$)

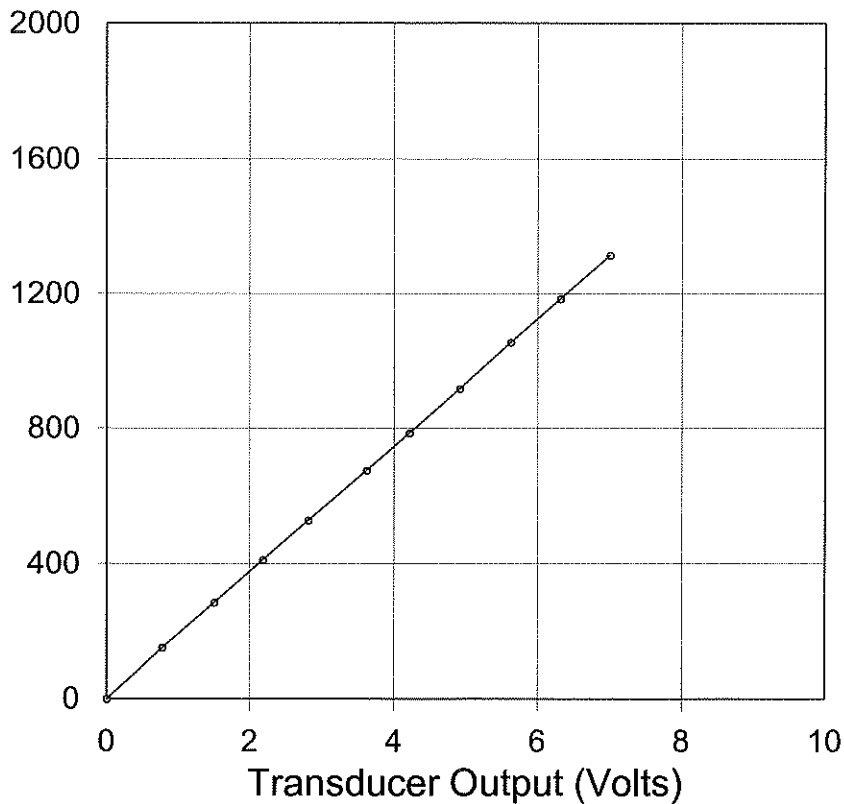

PDA Cal Factor (5.0 V)

93.6 $\mu\epsilon$ /V

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
152	0.77
286	1.50
410	2.18
527	2.81
675	3.61
785	4.21
917	4.91
1055	5.62
1186	6.31
1315	7.00

Shunt (60.4 K Ω)

2.5 V

General Factor

324.9 $\mu\epsilon$ /mV/V

Traceable to N.I.S.T.

Calibrated by: *George P. ...*

Calibrated on: 07-Sep-2010