




Pile Dynamics, Inc.

Transducer C030

Strain ($\mu\epsilon$)

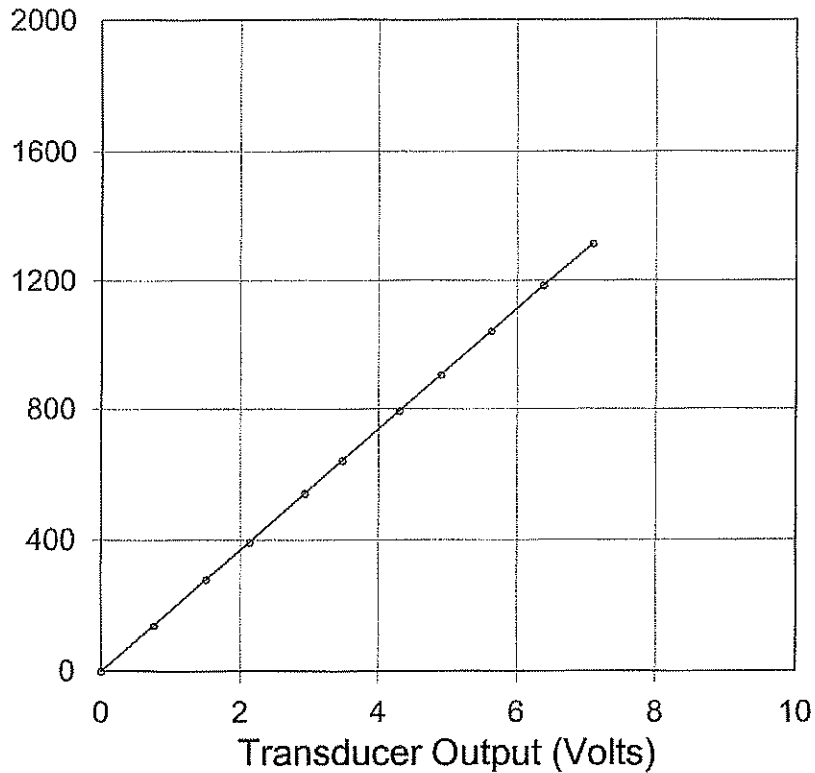

PDA Cal Factor (5.0 V)

92.8 $\mu\epsilon$ /V

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
139	0.75
281	1.50
392	2.13
541	2.93
641	3.47
794	4.30
905	4.89
1042	5.62
1186	6.37
1316	7.09

Shunt (60.4 K Ω)

2.5 V

General Factor

322.2 $\mu\epsilon$ /mV/V

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

Calibrated by:

Calibrated on:

08-Jan-2008