




# Pile Dynamics, Inc.

## Transducer C031

Strain ( $\mu\epsilon$ )

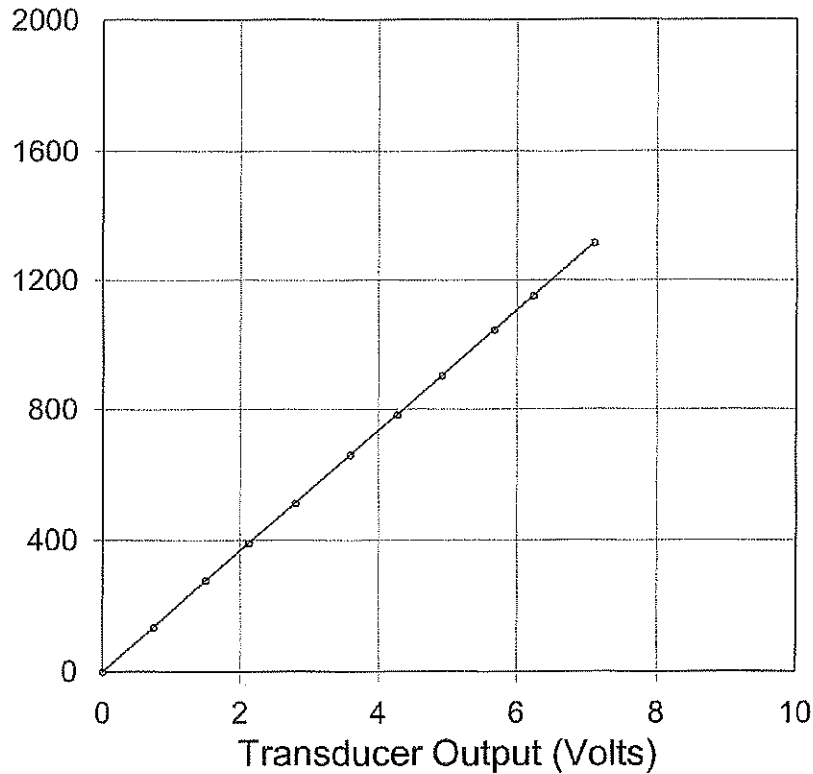

PDA Cal Factor (5.0 V)

92.3 $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
138	0.73
279	1.49
390	2.12
512	2.79
659	3.58
782	4.26
904	4.91
1044	5.66
1153	6.23
1317	7.10

Shunt (60.4 K $\Omega$ )

2.5 V

General Factor

320.5 $\mu\epsilon/mV/V$

Calibrated by:

Calibrated on:

03-Jan-2008

Traceable to N.I.S.T.