




# Pile Dynamics, Inc.

## Transducer C034

Strain ( $\mu\epsilon$ )

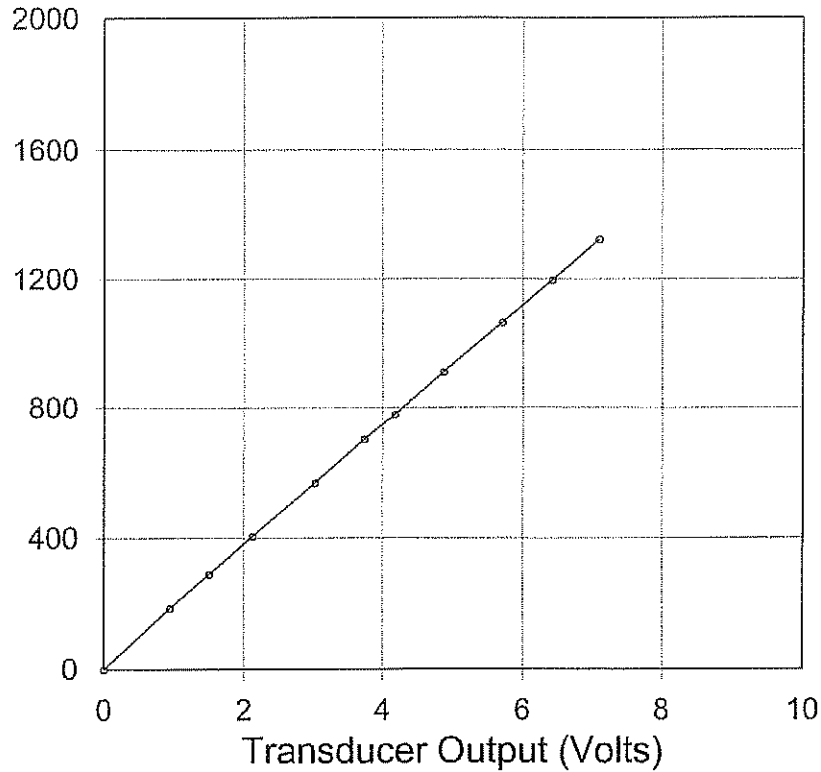

PDA Cal Factor (5.0 V)

92.7  $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
187	0.93
290	1.50
406	2.12
569	3.02
703	3.74
779	4.17
910	4.87
1067	5.70
1196	6.41
1323	7.09

Shunt (60.4 K $\Omega$ )

2.5 V

General Factor

322.0  $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

Calibrated by:

Calibrated on:

31-May-2008