




# Pile Dynamics, Inc.

## Transducer C037

Strain ( $\mu\epsilon$ )

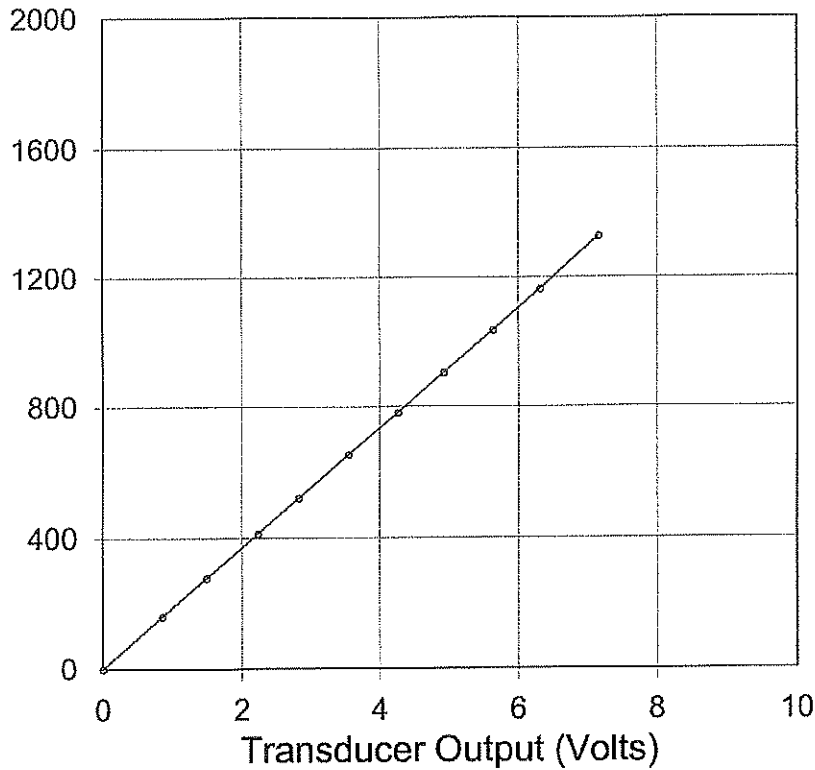

PDA Cal Factor (5.0 V)

92.0  $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
161	0.84
279	1.48
413	2.24
521	2.83
653	3.55
780	4.26
904	4.92
1036	5.63
1163	6.31
1329	7.17

Shunt (60.4 K $\Omega$ )

2.5 V

General Factor

319.4  $\mu\epsilon/mV/V$

Calibrated by:

Calibrated on:

07-Jan-2008

Traceable to N.I.S.T.