




Pile Dynamics, Inc.

Transducer C057

Strain ($\mu\epsilon$)

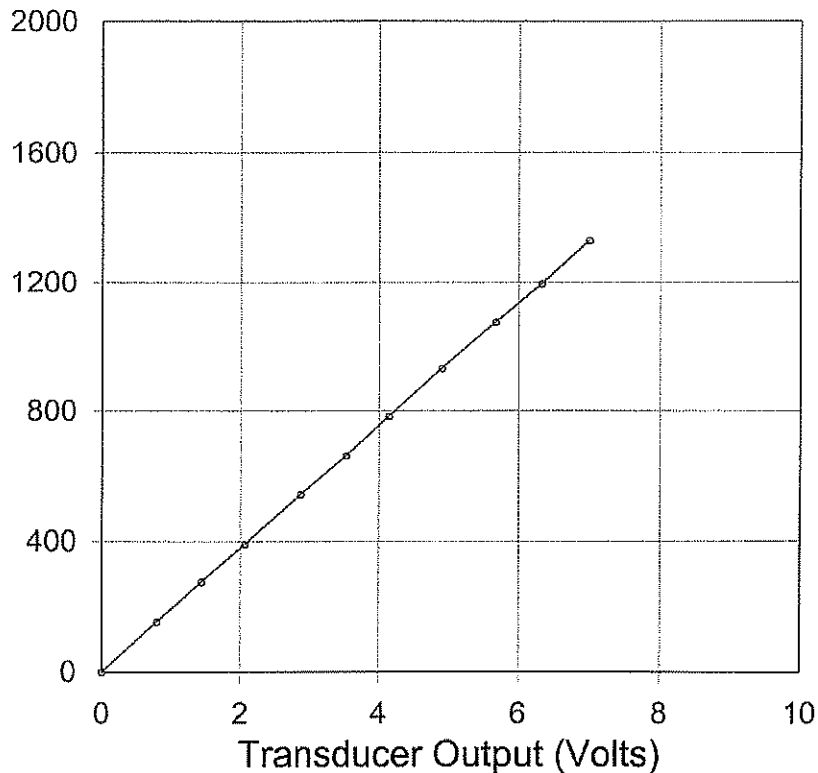

PDA Cal Factor (5.0 V)

94.7 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
154	0.79
276	1.43
391	2.06
543	2.86
662	3.52
782	4.14
931	4.90
1076	5.67
1196	6.32
1329	6.99

Shunt (60.4 K Ω)

2.5 V

General Factor

329.0 $\mu\epsilon/mV/V$

Calibrated by:

Katherine Miller

Calibrated on:

05-Dec-2007

Traceable to N.I.S.T.