


Pile Dynamics, Inc.

Transducer C058

Strain ($\mu\epsilon$)

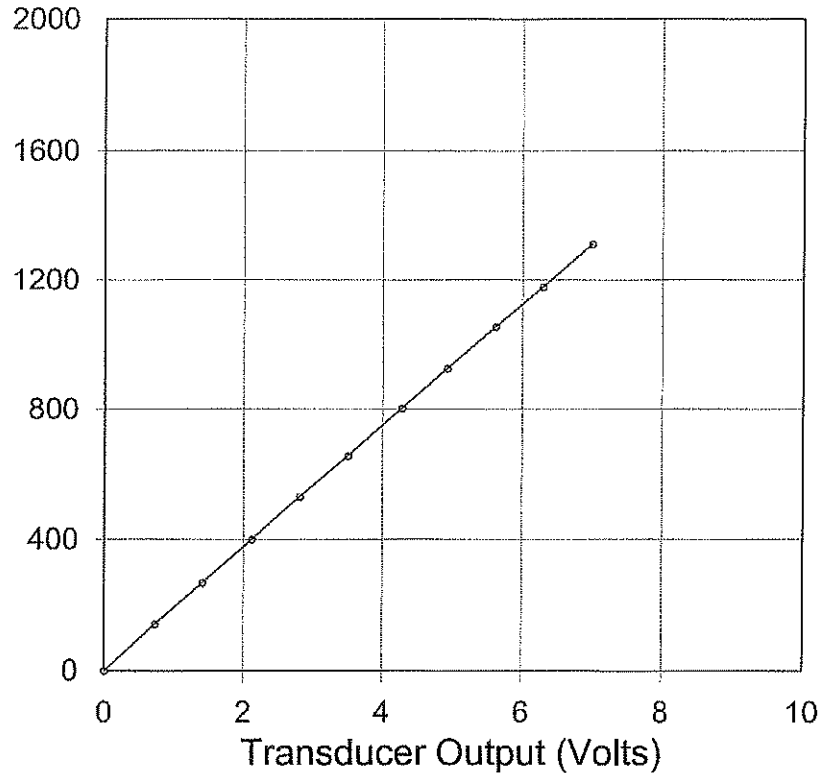

PDA Cal Factor (5.0 V)

93.6 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
142	0.72
267	1.40
400	2.12
530	2.81
656	3.50
802	4.27
925	4.92
1055	5.61
1179	6.29
1313	7.00

Shunt (60.4 K Ω)

2.5 V

General Factor

324.9 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Kaithe Billo

Calibrated on:

05-Dec-2007