




Pile Dynamics, Inc.

Transducer C060

Strain ($\mu\epsilon$)

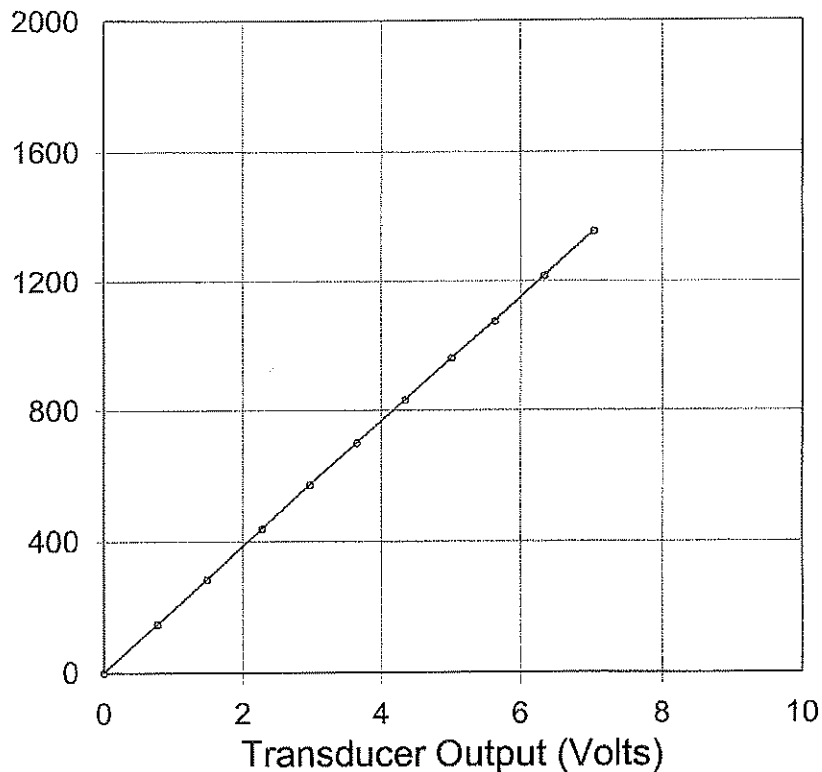

PDA Cal Factor (5.0 V)

96.0 $\mu\epsilon$ /V

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
149	0.76
284	1.47
439	2.27
572	2.96
700	3.64
832	4.34
962	5.01
1076	5.63
1218	6.33
1355	7.03

Shunt (60.4 K Ω)

2.5 V

General Factor

333.3 $\mu\epsilon$ /mV/V

Traceable to N.I.S.T.

Calibrated by: Kurtis Butler
 Calibrated on: 05-Dec-2007