




Pile Dynamics, Inc.

Transducer C062

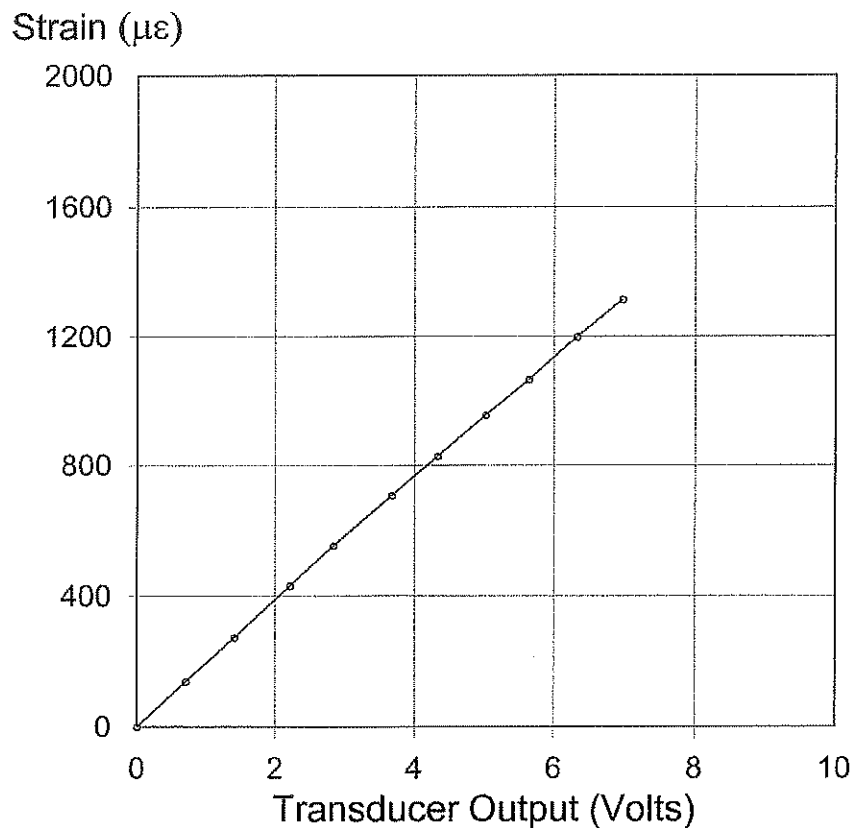

PDA Cal Factor (5.0 V) 94.2 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
139	0.70
274	1.40
430	2.21
553	2.84
707	3.67
828	4.33
955	5.01
1067	5.63
1200	6.32
1316	6.97

Shunt (60.4 K Ω) 2.5 V
 General Factor 326.9 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

Calibrated by: Kentley Heides
 Calibrated on: 05-Dec-2007