




Pile Dynamics, Inc.

Transducer C063

Strain ($\mu\epsilon$)

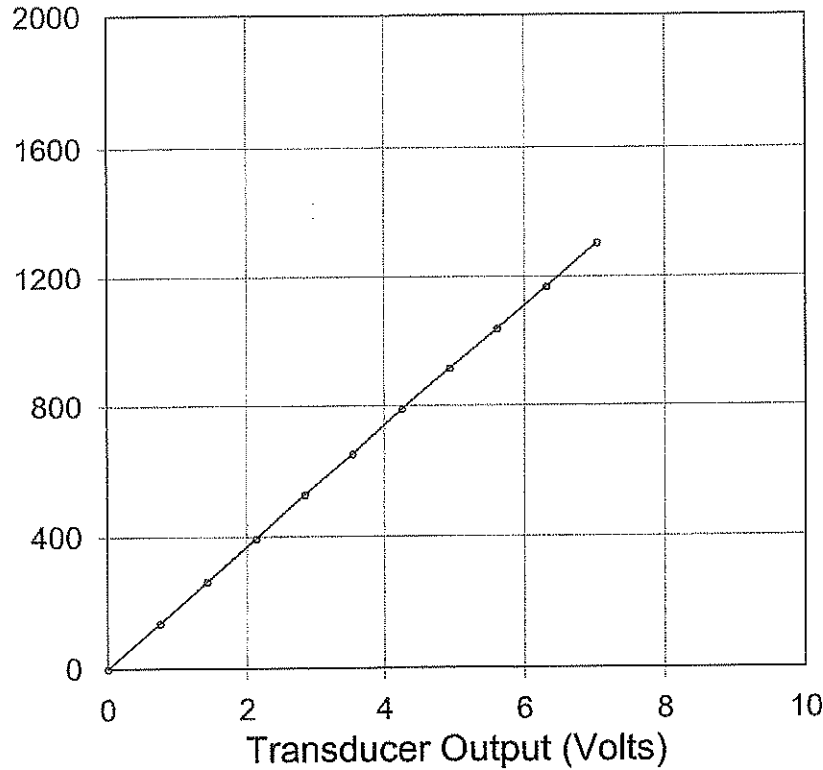

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

PDA Cal Factor (5.0 V)

92.6 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
140	0.73
264	1.42
393	2.13
527	2.84
651	3.54
789	4.25
915	4.93
1037	5.60
1168	6.31
1304	7.03

Shunt (60.4 K Ω)

2.5 V

General Factor

321.4 $\mu\epsilon/mV/V$

Calibrated by:

Kathleen Hillier

Calibrated on:

05-Dec-2007