




Pile Dynamics, Inc.

Transducer C064

Strain ($\mu\epsilon$)

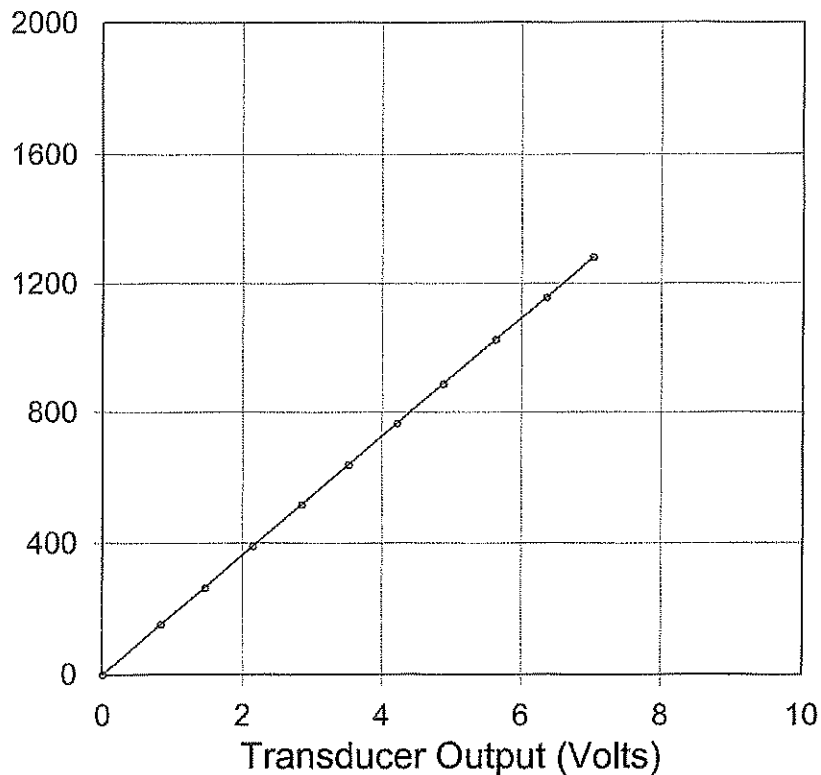

PDA Cal Factor (5.0 V)

91.1 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
156	0.83
265	1.45
391	2.14
516	2.84
637	3.51
765	4.21
886	4.87
1025	5.62
1158	6.35
1283	7.02

Shunt (60.4 K Ω)

2.5 V

General Factor

316.3 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Kurtz *W. Miller*

Calibrated on:

05-Dec-2007