




# Pile Dynamics, Inc.

## Transducer C077

Strain ( $\mu\epsilon$ )

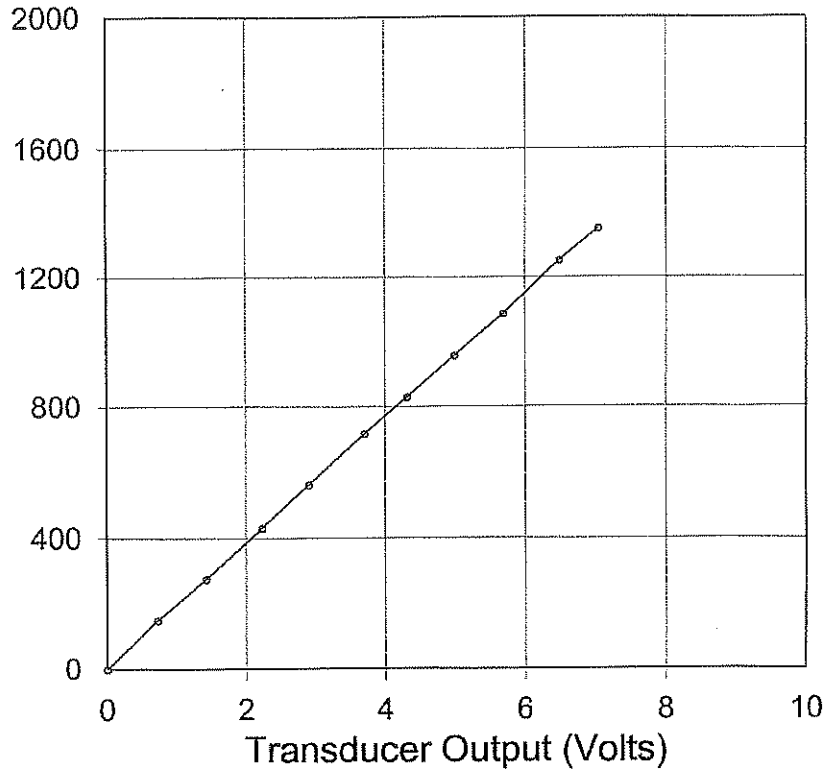

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

PDA Cal Factor (5.0 V)

95.7  $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
149	0.72
276	1.42
430	2.23
559	2.91
715	3.71
828	4.30
955	4.99
1086	5.68
1252	6.48
1351	7.04

Shunt (60.4 K $\Omega$ )

2.5 V

General Factor

332.3  $\mu\epsilon/mV/V$

Calibrated by:

*James A. Penteloff*

Calibrated on:

16-Sep-2009