




Pile Dynamics, Inc.

Transducer C079

Strain ($\mu\epsilon$)

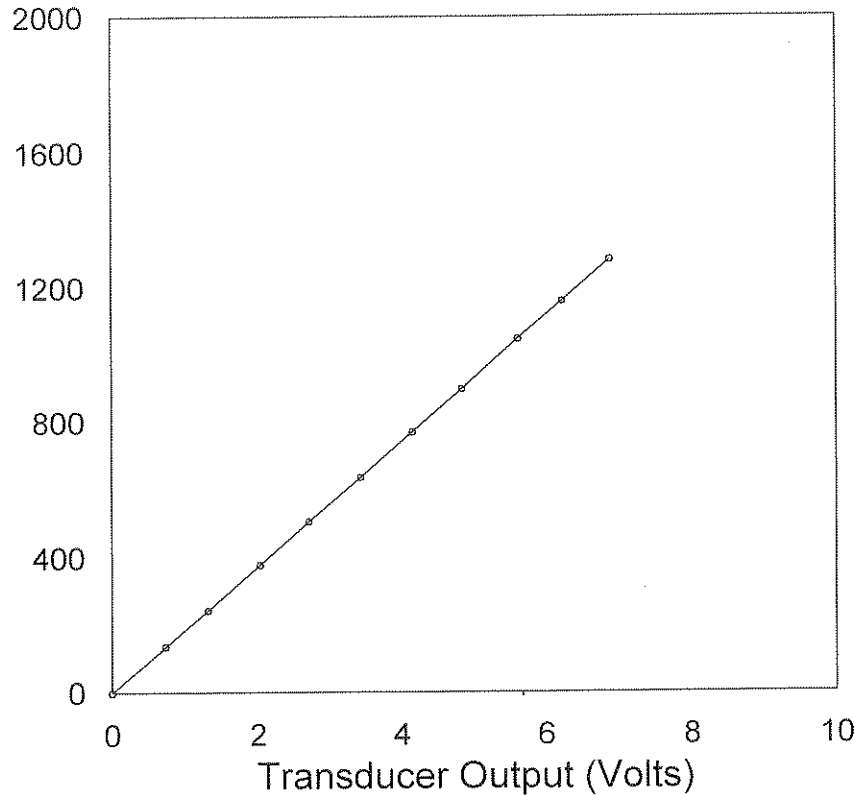

PDA Cal Factor (5.0 V)

93.1 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
137	0.72
244	1.31
377	2.02
504	2.71
635	3.43
769	4.15
897	4.84
1045	5.61
1160	6.21
1283	6.88

Shunt (60.4 K Ω)

2.5 V

General Factor

323.2 $\mu\epsilon/mV/V$

Calibrated by:

Calibrated on:

19-Aug-2011

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2009 Version 1.3

Smart Sensor? Yes No Smart Chip Programmed by: GP on: 19-August-2011 CRC value 3077