




Pile Dynamics, Inc.

Transducer C083

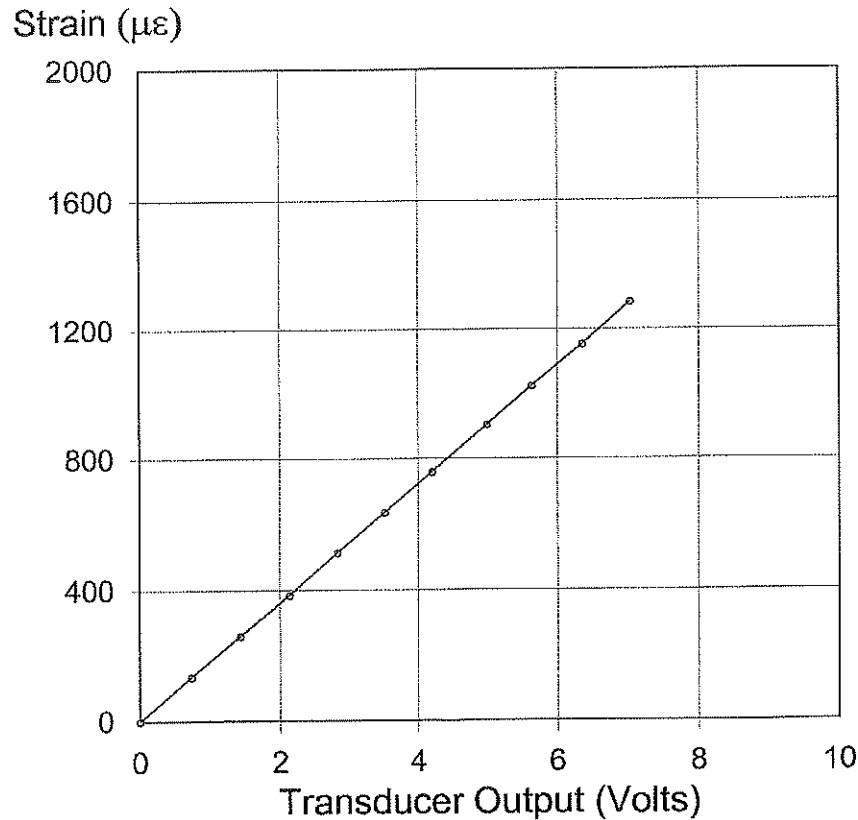


Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

PDA Cal Factor (5.0 V) 90.8 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
138	0.73
261	1.43
385	2.13
512	2.82
634	3.51
759	4.20
904	5.00
1022	5.63
1153	6.36
1285	7.03

Shunt (60.4 K Ω) 2.5 V
 General Factor 315.3 $\mu\epsilon/mV/V$

Calibrated by: 
 Calibrated on: 07-Jan-2008