




Pile Dynamics, Inc.

Transducer C105

Strain ($\mu\epsilon$)

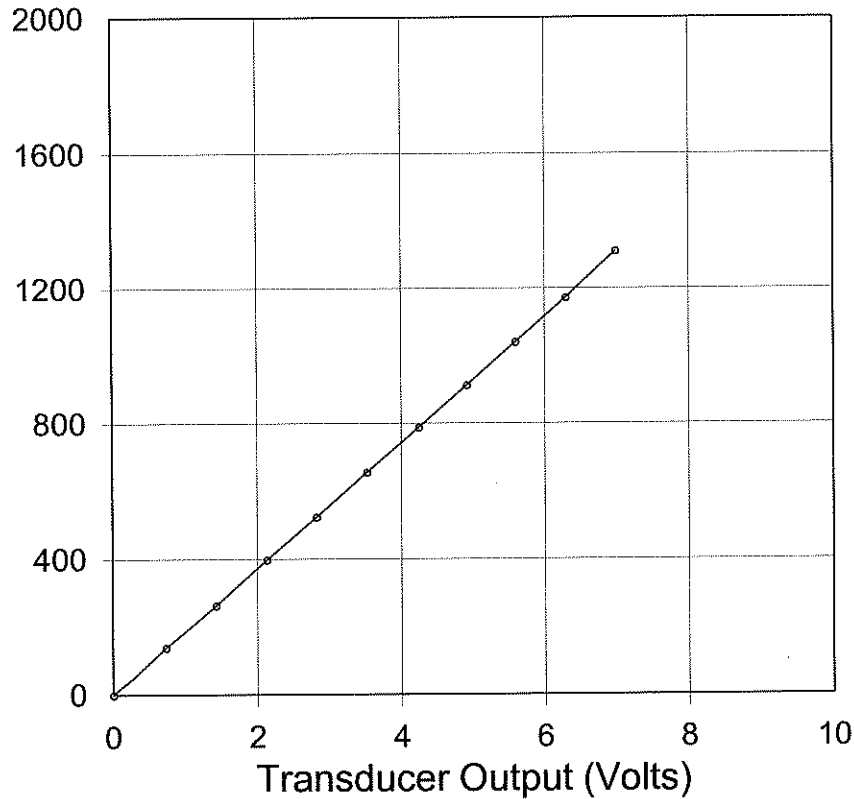

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2004 Version 1.2

PDA Cal Factor (5.0 V)

93.2 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
139	0.72
264	1.42
398	2.13
522	2.82
654	3.52
786	4.24
913	4.91
1040	5.59
1172	6.29
1311	6.99

Shunt (60.4 K Ω)
General Factor

2.5 V
323.8 $\mu\epsilon/mV/V$

Calibrated by:
Calibrated on:

Shael
06-Feb-2008