




# Pile Dynamics, Inc.

## Transducer C106

Strain ( $\mu\epsilon$ )

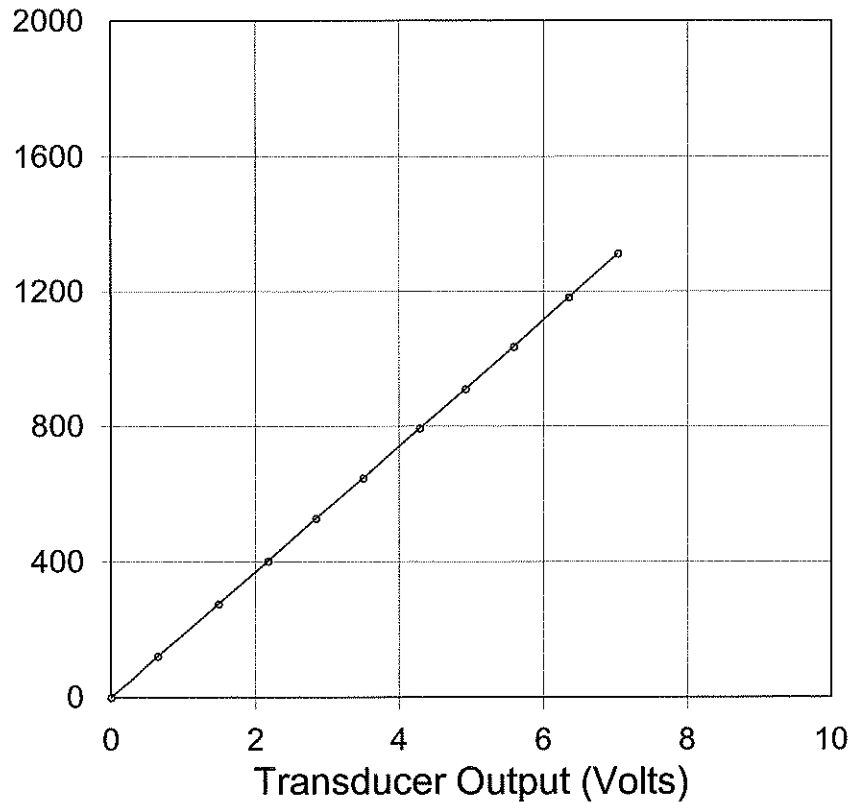

PDA Cal Factor (5.0 V)

93.1  $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
123	0.64
275	1.48
402	2.17
527	2.84
645	3.50
793	4.28
911	4.91
1036	5.58
1184	6.34
1313	7.03

Shunt (60.4 K $\Omega$ )

2.5 V

General Factor

323.4  $\mu\epsilon/mV/V$

Calibrated by:

Calibrated on:

06-Feb-2008

Traceable to N.I.S.T.