




Pile Dynamics, Inc.

# Pile Dynamics, Inc. Transducer C110

Strain ( $\mu\epsilon$ )

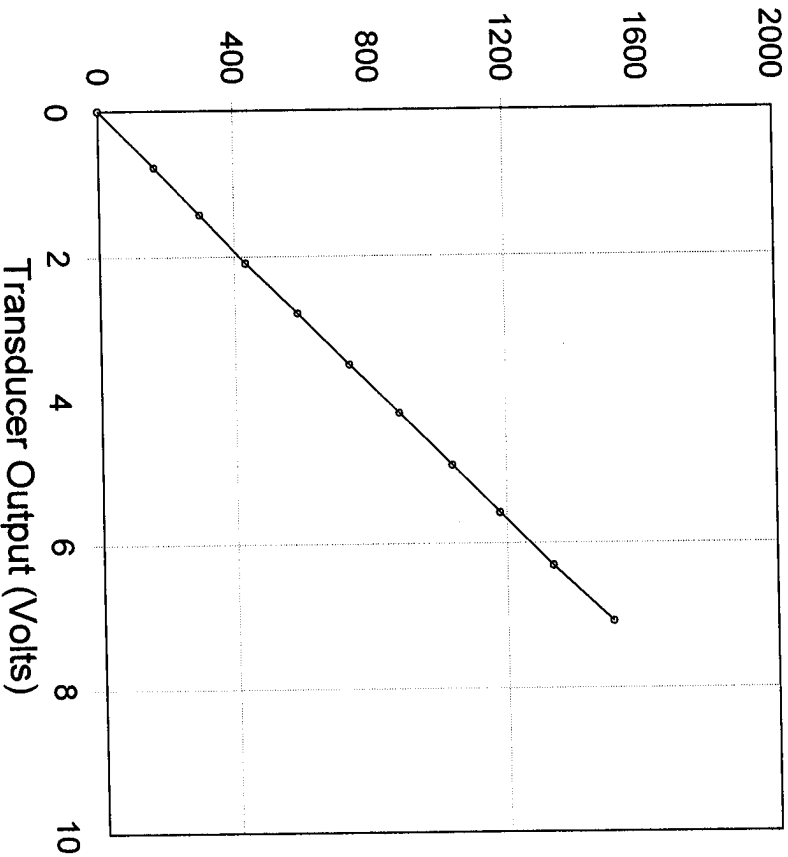

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

PDA Cal Factor (5.0 V)

106.4 $\mu\epsilon/V$

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
165	0.77
298	1.42
433	2.09
582	2.79
735	3.51
882	4.19
1037	4.92
1178	5.58
1338	6.31
1513	7.08

Shunt (60.4 K $\Omega$ )

2.5 V

General Factor

369.4 $\mu\epsilon/mV/V$

Calibrated by:

Calibrated on:

18-Apr-2014