




Pile Dynamics, Inc.

Pile Dynamics, Inc. Transducer C111

Strain ($\mu\epsilon$)

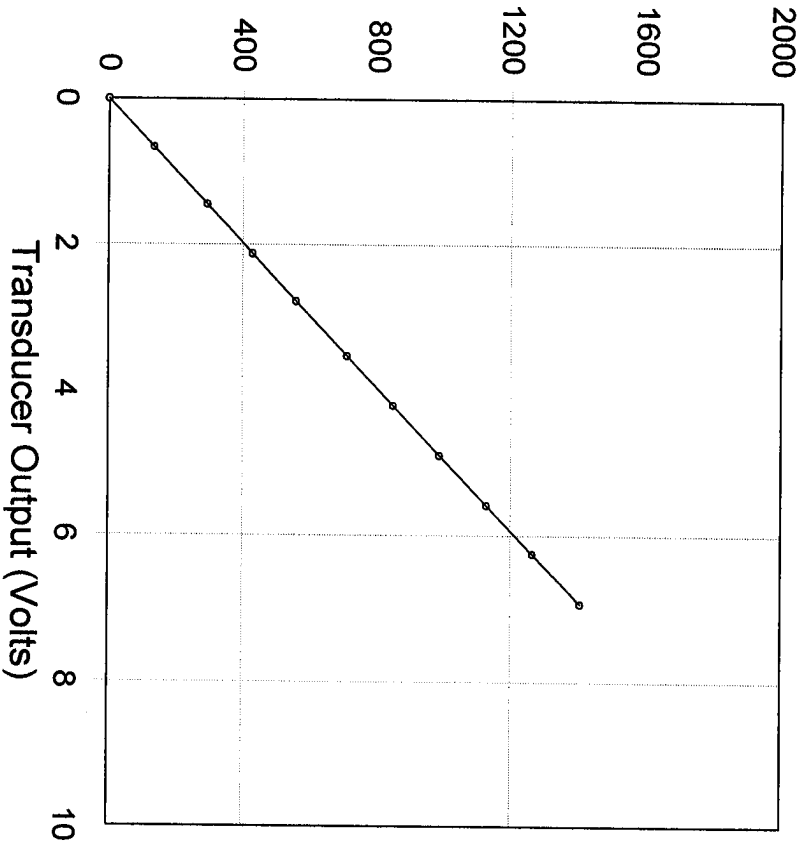

PDA Cal Factor (5.0 V)

101.1 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
135	0.66
293	1.44
428	2.12
558	2.77
708	3.52
848	4.20
985	4.89
1126	5.58
1266	6.25
1408	6.94

Shunt (60.4 K Ω)

2.5 V

General Factor

351.2 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Strain Transducer Calibrator System 2011 Version 1.5

Calibrated by:
Calibrated on:


18-Apr-2014