




# Pile Dynamics, Inc.

## Transducer C120

Strain ( $\mu\epsilon$ )

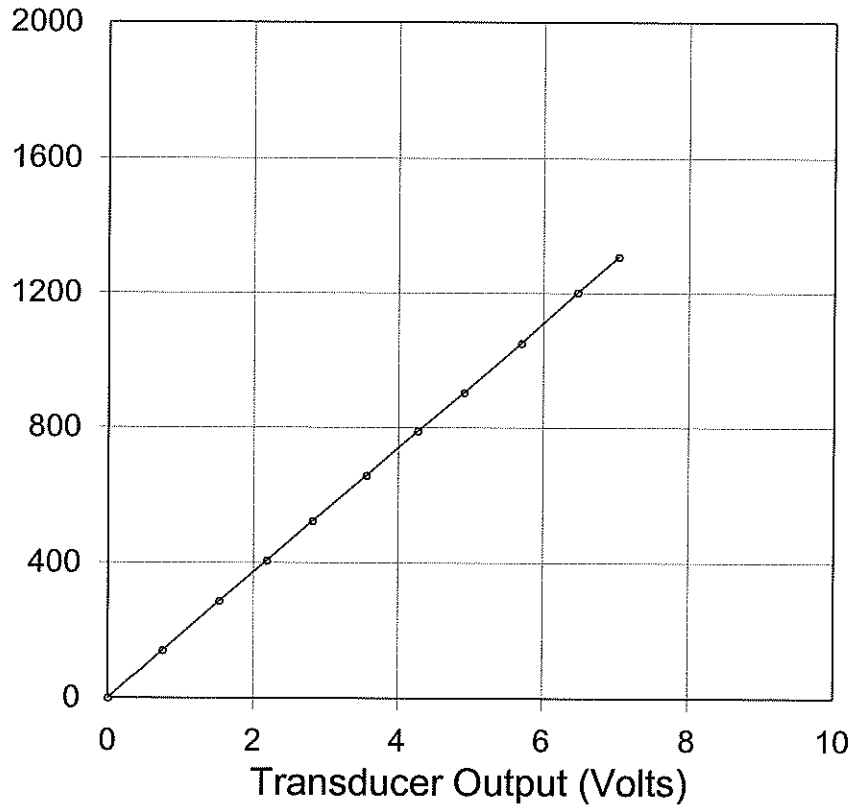

PDA Cal Factor (5.0 V)

92.6 $\mu\epsilon$ /V

Applied Strain ( $\mu\epsilon$ )	Transducer Output (Volts)
0	0.00
141	0.74
287	1.52
407	2.18
522	2.81
657	3.55
788	4.26
904	4.90
1052	5.69
1202	6.46
1309	7.03

Shunt (60.4 K $\Omega$ )

2.5 V

General Factor

321.5 $\mu\epsilon$ /mV/V

Calibrated by:

Calibrated on:

06-Feb-2008

Traceable to N.I.S.T.