




Pile Dynamics, Inc.

Transducer C123

Strain ($\mu\epsilon$)

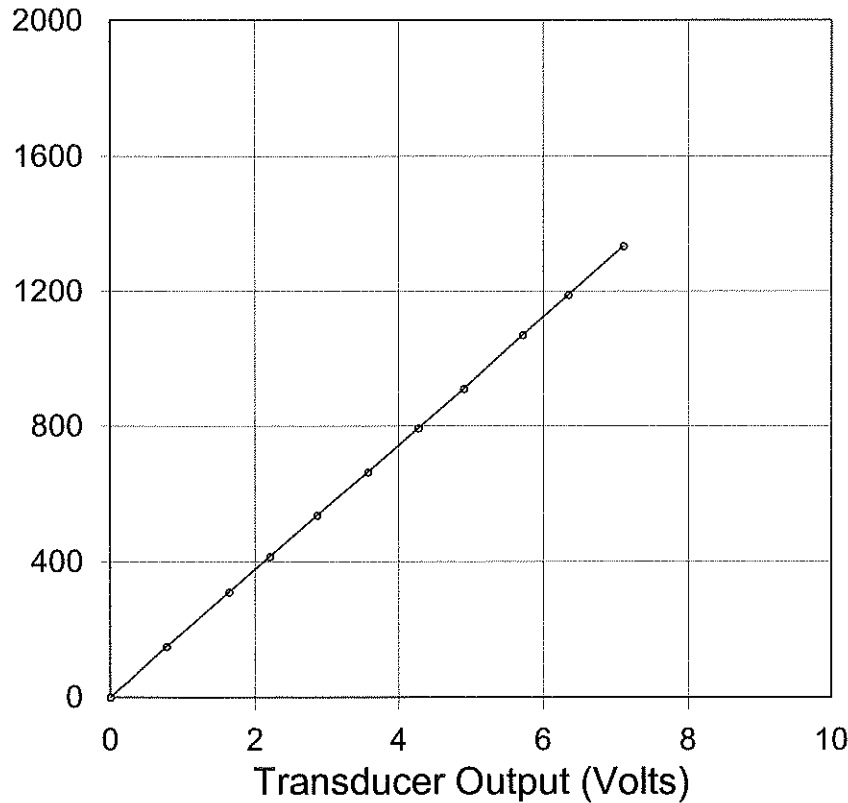

PDA Cal Factor (5.0 V)

93.4 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
150	0.76
311	1.64
415	2.20
535	2.86
664	3.57
793	4.27
910	4.89
1069	5.71
1189	6.34
1334	7.10

Shunt (60.4 K Ω)

2.5 V

General Factor

324.2 $\mu\epsilon/mV/V$

Calibrated by:

Calibrated on:

21-Nov-2008

Traceable to N.I.S.T.