




Pile Dynamics, Inc.

Transducer C124

Strain ($\mu\epsilon$)

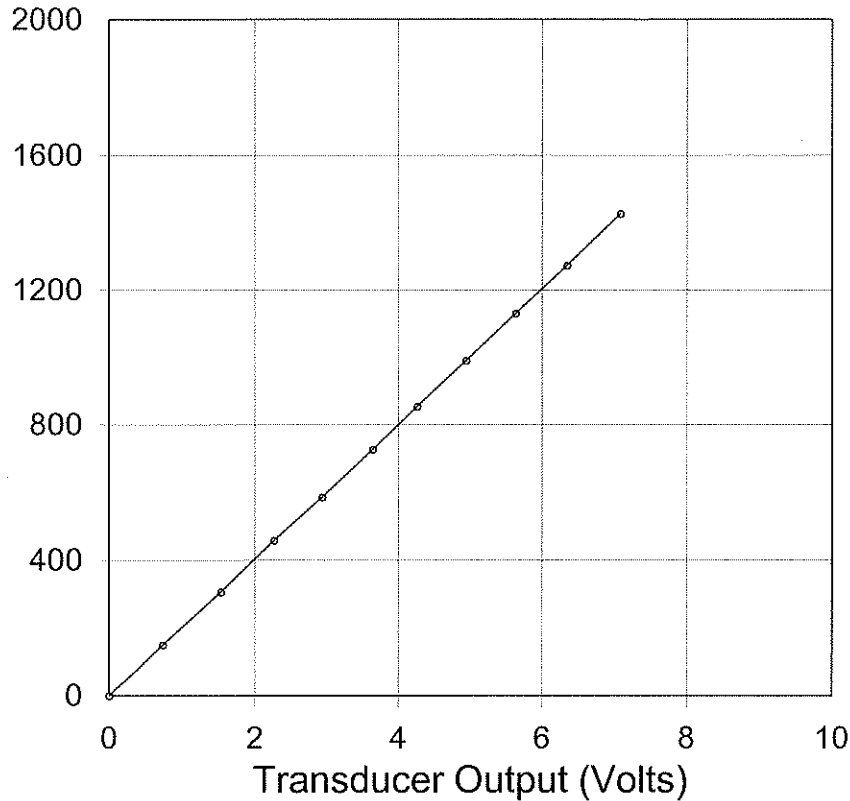

PDA Cal Factor (5.0 V)

100.5 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
150	0.72
307	1.52
457	2.26
586	2.93
727	3.64
854	4.26
990	4.94
1131	5.63
1274	6.34
1429	7.08

Shunt (60.4 K Ω)

2.5 V

General Factor

348.9 $\mu\epsilon/mV/V$

Calibrated by:

Calibrated on:

09-Jun-2008

Traceable to N.I.S.T.