




Pile Dynamics, Inc.

Transducer C125

Strain ($\mu\epsilon$)

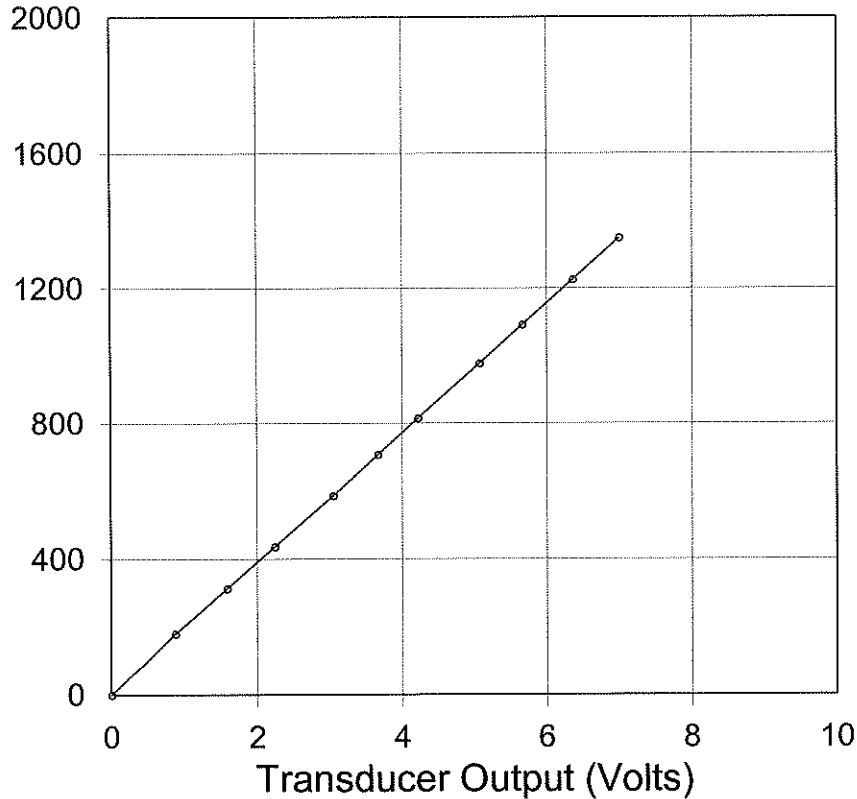

PDA Cal Factor (5.0 V)

95.9 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
181	0.87
313	1.58
436	2.24
586	3.04
707	3.67
816	4.22
978	5.07
1091	5.66
1226	6.36
1349	7.00

Shunt (60.4 K Ω)

2.5 V

General Factor

332.8 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by: *Garry Pinnick*

Calibrated on: 19-Nov-2008