




Pile Dynamics, Inc.

Transducer C126

Strain ($\mu\epsilon$)

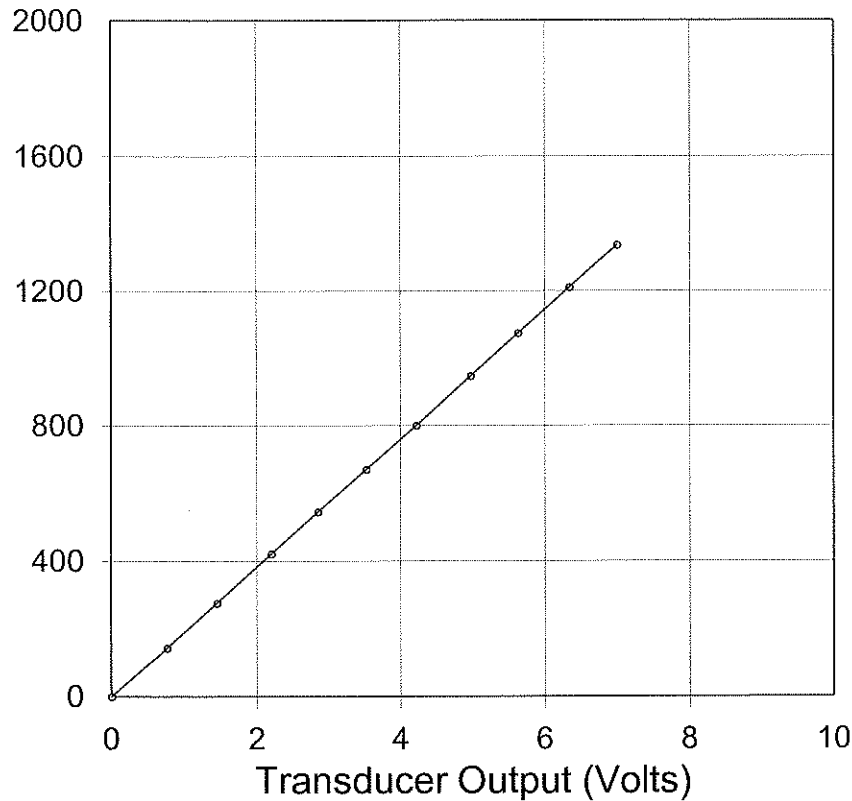

PDA Cal Factor (5.0 V)

95.3 $\mu\epsilon/V$

Applied Strain ($\mu\epsilon$)	Transducer Output (Volts)
0	0.00
143	0.74
277	1.44
420	2.20
545	2.85
669	3.52
801	4.22
946	4.97
1075	5.63
1211	6.34
1336	7.00

Shunt (60.4 K Ω)

2.5 V

General Factor

331.0 $\mu\epsilon/mV/V$

Traceable to N.I.S.T.

Calibrated by:

Calibrated on:

10-Jun-2008